

Greymouth Petroleum Turangi Ltd
Turangi-B Hydraulic Fracturing
Monitoring Programme
Annual Report
2021-2023
Technical Report 2024-65



Greymouth Petroleum Turangi Ltd
Turangi-B Hydraulic Fracturing
Monitoring Programme
Annual Report
2021-2023
Technical Report 2024-65

Taranaki Regional Council
Private Bag 713
Stratford

ISSN: 1178-1467 (Online)
Document: 3282123 (Word)
Document: 3303935 (Pdf)
October 2024

Executive summary

Greymouth Petroleum Turangi Ltd (the Company) operates the Turangi-B hydrocarbon exploration site (wellsite) located on Turangi Road, Tikorangi located in the Parahaki catchment. This report outlines and discusses the results of the monitoring programme implemented by the Council in relation to hydraulic fracturing activities conducted by the Company at the wellsite over the period 23 July 2021 to 8 June 2023. The report also details the results of the monitoring undertaken and assesses the environmental effects of the Company's activities.

The programme of hydraulic fracturing undertaken by the Company at the Turangi-B wellsite included the hydraulic fracturing of five wells. The wells targeted for stimulation were the Turangi-11, Turangi-18, Turangi-16, Turangi-14 and Turangi-19 wells.

During the monitoring period, the Company demonstrated an overall high level of environmental and a high level of administrative performance.

The programme of monitoring implemented by the Council in relation to these hydraulic fracturing activities spanned the 2021/22 and 2022/23 monitoring years. Monitoring included pre and post-discharge groundwater sampling in relation to discharges at the Turangi-B wellsite. In order to characterise the discharges and to determine compliance with consent conditions samples of hydraulic fracturing fluids, and fluids returning to the wellhead post-fracturing, were also collected by the Company and results of the physicochemical analysis undertaken were provided to the Council. This is the third monitoring report produced by the Council in relation to the hydraulic fracturing activities at the Turangi-B wellsite.

The monitoring carried out by the Council indicates that the hydraulic fracturing activities undertaken by the Company had no significant adverse effects on local groundwater or surface water resources. There were no unauthorised incidents recording non-compliance in respect of the resource consent held by the Company in relation to these activities or provisions in regional plans, during the period under review.

For reference, in the 2021/22 year, consent holders were found to achieve a high level of environmental performance and compliance for 88% of the consents monitored through the Taranaki tailored monitoring programmes, while for another 10% of the consents, a good level of environmental performance and compliance was achieved.

For reference, in the 2022/23 year, consent holders were found to achieve a high level of environmental performance and compliance for 878 (87%) of a total of 1007 consents monitored through the Taranaki tailored monitoring programmes, while for another 96 (10%) of the consents a good level of environmental performance and compliance was achieved. A further 27 (3%) of consents monitored required improvement in their performance, while the remaining one (<1%) achieved a rating of poor.

This report includes recommendations for the future monitoring of any hydraulic fracturing activities at the Turangi-B wellsite.

Table of contents

	Page	
1.	Introduction	1
1.1	Compliance monitoring programme reports and the Resource Management Act 1991	1
1.1.1	Introduction	1
1.1.2	Structure of this report	1
1.1.3	The Resource Management Act 1991 and monitoring	1
1.1.4	Evaluation of environmental performance	2
1.2	Process description	2
1.2.1	Hydraulic fracturing	2
1.2.2	The Turangi-B wellsite and hydraulic fracturing activities	3
1.3	Resource consents	6
1.4	Monitoring programme	6
1.4.1	Introduction	6
1.4.2	Programme liaison and management	6
1.4.3	Assessment of data submitted by the consent holder	6
1.4.4	Physicochemical sampling	7
1.4.5	Surface water quality monitoring	8
2.	Results	9
2.1	Physicochemical sampling	9
2.1.1	Groundwater	9
2.2	Consent holder submitted data	12
2.2.1	Turangi-11 post fracturing discharge report	12
2.2.2	Turangi-14 post fracturing discharge report	12
2.2.3	Turangi-16 post fracturing discharge report	12
2.2.4	Turangi-18 post fracturing discharge report	13
2.2.5	Turangi-19 post fracturing discharge report	13
2.2.6	Hydraulic fracturing and return fluids	14
2.3	Incidents, investigations, and interventions	17
3.	Discussion	18
3.1	Environmental effects of exercise of consent	18
3.2	Evaluation of performance	18
3.3	Recommendations from the 2019-2021 Report	19
3.4	Alterations to monitoring programmes for future hydraulic fracturing activities	20

4.	Recommendations	21
	Glossary of common terms and abbreviations	22
	Bibliography and references	24
Appendix I	Resource consent held by Greymouth Petroleum Turangi Ltd	
Appendix II	Categories used to evaluate environmental and administrative performance	
Appendix III	Certificates of analysis (groundwater)	
Appendix IV	Certificates of analysis (hydraulic fracturing fluids)	

List of tables

Table 1	Summary of hydraulic fracturing details	4
Table 2	Resource consent held by the Company during the period under review	6
Table 3	Details of groundwater sites included in the monitoring programme	7
Table 4	Details of surface water sites included in the monitoring programme	8
Table 5	Results of groundwater sampling carried out in relation to the Turangi-B fracturing events	10
Table 6	Results of hydraulic fracturing fluid sampling	15
Table 7	Results of hydraulic fracturing return fluid sampling	15
Table 8	Summary of performance for consent 7952-2	18
Table 9	Evaluation of environmental performance over time)	19

List of figures

Figure 1	Location map	5
----------	--------------	---

1. Introduction

1.1 Compliance monitoring programme reports and the Resource Management Act 1991

1.1.1 Introduction

This report outlines and discusses the results of the monitoring programme implemented by Taranaki Regional Council (the Council) in relation to the programme of hydraulic fracturing undertaken by Greymouth Petroleum Turangi Ltd (the Company) at the Turangi-B wellsite, over the period 23 July 2021 to 8 June 2023. The report also assesses the Company's level of environmental performance and compliance with the resource consent held in relation to the activity.

The programme of hydraulic fracturing undertaken by the Company at the Turangi-B wellsite included the hydraulic fracturing of five wells. The wells targeted for stimulation were the Turangi-11, Turangi-18, Turangi-16, Turangi-14 and Turangi-19 wells.

The programme of monitoring implemented by the Council in relation to these hydraulic fracturing activities spanned the 2021/22 and 2022/23 monitoring years. Monitoring included a mixture of groundwater, surface water and discharge monitoring components. This is the third monitoring report produced by the Council in relation to hydraulic fracturing activities at the Turangi-B wellsite.

1.1.2 Structure of this report

Section 1 of this report is a background section. It sets out general information about:

- consent compliance monitoring under the *Resource Management Act 1991* (RMA) and the Council's obligations;
- the Council's approach to monitoring sites through compliance monitoring programmes;
- the resource consents held by the Company;
- the nature of the monitoring programme in place for the period under review; and
- a description of the activities and operations conducted at the Turangi-B wellsite.

Section 2 presents the results of monitoring during the period under review, including scientific and technical data.

Section 3 discusses the results, their interpretations, and their significance for the environment.

Section 4 presents recommendations to be implemented for the future monitoring of any hydraulic fracturing activities at the Turangi-B wellsite.

A glossary of common abbreviations and scientific terms, and a bibliography, are presented at the end of the report.

1.1.3 The Resource Management Act 1991 and monitoring

The RMA primarily addresses environmental 'effects' which are defined as positive or adverse, temporary or permanent, past, present or future, or cumulative. Effects may arise in relation to:

- a. the neighbourhood or the wider community around an activity, and may include cultural and social-economic effects;
- b. physical effects on the locality, including landscape, amenity and visual effects;

- c. ecosystems, including effects on plants, animals, or habitats, whether aquatic or terrestrial;
- d. natural and physical resources having special significance (for example recreational, cultural, or aesthetic); and
- e. risks to the neighbourhood or environment.

In drafting and reviewing conditions on discharge permits, and in implementing monitoring programmes, the Council is recognising the comprehensive meaning of 'effects' in as much as is appropriate for each activity. Monitoring programmes are not only based on existing permit conditions, but also on the obligations of the RMA to assess the effects of the exercise of consents. In accordance with Section 35 of the RMA, the Council undertakes compliance monitoring for consents and rules in regional plans, and maintains an overview of the performance of resource users and consent holders. Compliance monitoring, including both activity and impact monitoring, enables the Council to continually re-evaluate its approach and that of consent holders to resource management and, ultimately, through the refinement of methods and considered responsible resource utilisation, to move closer to achieving sustainable development of the region's resources.

1.1.4 Evaluation of environmental performance

Besides discussing the various details of the performance and extent of compliance by the consent holders, this report also assigns a rating as to each Company's environmental and administrative performance during the period under review. The rating categories are high, good, improvement required and poor for both environmental and administrative performance. The interpretations for these ratings are found in Appendix II.

For reference, in the 2021/22 year, consent holders were found to achieve a high level of environmental performance and compliance for 88% of the consents monitored through the Taranaki tailored monitoring programmes, while for another 10% of the consents, a good level of environmental performance and compliance was achieved.

For reference, in the 2022/23 year, consent holders were found to achieve a high level of environmental performance and compliance for 878 (87%) of a total of 1007 consents monitored through the Taranaki tailored monitoring programmes, while for another 96 (10%) of the consents a good level of environmental performance and compliance was achieved. A further 27 (3%) of consents monitored required improvement in their performance, while the remaining one (<1%) achieved a rating of poor.¹

1.2 Process description

1.2.1 Hydraulic fracturing

Hydraulic fracturing is a reservoir stimulation technique used to increase the flow of hydrocarbons to the surface. The primary objective of hydraulic fracturing is to increase the permeability of the target reservoir by creating numerous small, interconnected fractures, thus increasing the flow of hydrocarbons from the formation to a given well. The process of hydraulic fracturing has enabled companies to produce hydrocarbons at economically viable rates from extremely low permeability reservoirs and those that have become depleted using conventional production techniques.

¹ The Council has used these compliance grading criteria for more than 20 years. They align closely with the 4 compliance grades in the MfE Best Practice Guidelines for Compliance, Monitoring and Enforcement, 2018

The process of hydraulic fracturing involves the pumping of fluids and a proppant (medium-grained sand or small ceramic pellets) down a well, through a perforated section of the well casing, and into the target reservoir. The fluid mixture is pumped at a pressure that exceeds the fracture strength of the reservoir rock in order to create fractures. Once fractures have been initiated, pumping continues in order to force the fluid and proppant into the fractures created. The proppant is designed to keep the fractures open when the pumping is stopped. The placement of proppant into the fractures can be assisted by the use of cross-linked gels (gel fracturing), turbulent flow (slick-water fracturing), or the use of nitrogen gas.

1.2.1.1 Gel fracturing

Gel fracturing utilises cross-linked gel solutions, which are liquid at the surface but, when mixed, form long-chain polymer bonds and thus become viscous gels. These gels are used to transport the proppant into the formation. Once in the formation they 'break' back with time, temperature and the aid of gel breaking chemicals into a liquid state and are flowed back to surface, without disturbing the proppant which remains in place and enhances the flow of hydrocarbons back to the surface.

1.2.1.2 Slick water fracturing

Slick water fracturing utilises water based fracturing fluids with friction-reducing additives. The addition of the friction reducers allows the fracturing fluids and proppant to be pumped to the target zone at higher rates and reduced pressures, than when using water alone. The higher rate creates turbulence within the fluid column holding the proppant and enabling its placement into the open fractures and enhancing the flow of hydrocarbons back to the surface.

1.2.1.3 Nitrogen gas fracturing

Nitrogen gas assisted fracturing involves replacing some of the fluid used in the fracturing process with nitrogen gas, which can fracture rock at high pressures much like water. While nitrogen (N₂) is a gas at room temperature, it can be maintained in a liquid state through cooling and pressurisation. Nitrogen assisted fracturing can be beneficial from a production standpoint as inevitably during the fracturing process some of the water pumped down the well remains underground in the rock formation, which can block some of the small pores, inhibiting hydrocarbon recovery. The use of nitrogen gas reduces the amount of water required for each fracturing event. This also reduces the total concentration of chemical additives required and the volume of water returning to the surface that requires subsequent disposal.

1.2.2 The Turangi-B wellsite and hydraulic fracturing activities

The Turangi-B wellsite is located on Turangi Road Upper near Waitara and lies within the Parahaki catchment. The area surrounding the site is rural in nature and farming and forestry activities co-exist with active petroleum exploration and production operations. The location of the wellsite is illustrated in Figure 1. A summary of the hydraulic fracturing activities carried out by the Company at the Turangi-B wellsite during the period being reported is provided below in Table 1.

Table 1 Summary of hydraulic fracturing details

Well	Bore id.	Date range	Mid-point injection intervals (m TVDss)	Formation
Turangi-11	GND3110	23/07/2021–17/11/2022	3,404.8–3,418	Mangahewa/Kaimiro
Turangi-14	GND3163	2/9/2021–8/9/2021	3,954–4,074	
Turangi-16	GND3164	24/3/2022–19/5/2022	3,415–4,538	
Turangi-18	GND3232	5/12/2022–1/2/2023	3,421–4,036	
Turangi-19	GND3231	28/4/2023–8/6/2023	3419.9–4084.4	



Figure 1 Location map

1.3 Resource consents

The Company holds one resource consent the details of which is summarised in Table 2 below. Summaries of the conditions attached to the permit are set out in Section 3 of this report.

A summary of the various consent types issued by the Council is included in Appendix I, as is a copy of the permit held by the Company during the period under review.

Table 2 Resource consent held by the Company during the period under review

Consent number	Purpose of consent	Granted	Next review	Expires
7952-2	To discharge water based hydraulic fracturing fluids into land at depths greater than 3,410m TVDss beneath the Turangi-B wellsite	9 June 2016	June 2024	01 June 2033

1.4 Monitoring programme

1.4.1 Introduction

Section 35 of the RMA sets obligations upon the Council to gather information, monitor and conduct research on the exercise of resource consents within the Taranaki region. The Council is also required to assess the effects arising from the exercising of these consents and report upon them.

The Council may therefore make and record measurements of physical and chemical parameters, take samples for analysis, carry out surveys and inspections, conduct investigations and seek information from consent holders.

The monitoring programme for the Turangi-B wellsite consisted of four primary components.

1.4.2 Programme liaison and management

There is generally a significant investment of time and resources by the Council in:

- ongoing liaison with resource consent holders over consent conditions and their interpretation and application;
- discussion over monitoring requirements;
- preparation for any consent reviews, renewals or new consent applications;
- advice on the Council's environmental management strategies and content of regional plans; and
- consultation on associated matters.

1.4.3 Assessment of data submitted by the consent holder

As required by the conditions of consent 7952, the Company submitted pre and post fracturing discharge reports to the Council for each well fractured during the period under review. Pre-fracturing discharge reports provide an outline of the proposed fracturing operations in relation to each well, while post fracturing reports confirm details of what actually occurred. The specific range of information required in each report is stipulated in the conditions of the consent.

1.4.4 Physicochemical sampling

1.4.4.1 Groundwater

As a general principle, all existing bores or wells within a 1km radius of a hydraulic fracturing activity are assessed for their suitability for sampling (or otherwise) and included in the monitoring programme for the wellsite.

The survey of existing sites resulted in a total of 15 potential groundwater sampling locations being identified. Assessment of the sites indicated that they were all either greater than 500m from the wellsite or were very shallow monitoring bores, previously installed by the company for monitoring various activities onsite.

As there were no suitable monitoring sites identified, consent conditions required the Company to install a site specific monitoring bore. The new bore installed by the Company is the sole groundwater monitoring site included in the monitoring programme. A summary of bore details are included in Table 3 below.

Samples of groundwater were obtained pre-fracturing to provide a baseline reference of groundwater composition and a further seven rounds of sampling were carried out during and following completion of the activities.

Groundwater samples are collected following standard groundwater sampling methodologies and generally in accordance with the National Environmental Monitoring Standards (NEMS) for discrete groundwater quality sampling (2019). All samples were transported to Hill Laboratories Ltd (Hills) for analysis following standard chain of custody procedures.

Table 3 Details of groundwater sites included in the monitoring programme

Monitoring site	Easting (NZTM)	Northing (NZTM)	Distance from wellsite (m)	Total depth (m)	Screened/open interval (m)	Aquifer
GND3061	1713538	5682554	<50	33	23-32	Marine terraces north

1.4.4.2 Hydraulic fracturing and return fluids

In addition to the sampling of local groundwater, representative samples of the hydraulic fracturing fluid and reservoir fluids produced back to the wellhead immediately following each fracturing event (return fluids) are obtained for analysis.

Samples of return fluids were collected at regular intervals during the flow-back period. Return fluids are comprised of a mixture of hydraulic fracturing fluids and formation fluids produced from the target reservoir, following the completion of the hydraulic fracturing process. The relative concentrations of each contributing fluid type change as the volume of fluid produced from the well increases. Immediately following the opening of the well post fracturing, a high proportion of the fluid returning to the wellhead is fluid injected during the hydraulic fracturing process. As the volume of fluid produced from the well increases, the proportion of hydraulic fracturing fluid reduces in relation to formation fluids. The individual samples of return fluid are generally combined in a composite sample for laboratory analysis. Composites are designed to provide a representative sample of fluids returning to the wellhead over the entire flow-back period.

All samples are collected and sent by the Company to Hills for analysis. Results are provided to the Council on request or in the post fracturing report provided following each fracturing event.

1.4.5 Surface water quality monitoring

The Parahaki Stream is located to the south west of the Turangi-B wellsite (Figure 1). Following a survey of the area no suitable surface water monitoring sites were identified down-gradient of the well site discharges and the estimated location of groundwater/subsurface drainage from the discharge area. Therefore no surface water monitoring was required for inclusion in the Hydraulic Fracturing monitoring programme.

Following a temporary change in wellsite discharge from land to water at the wellsite, three surface water sampling sites were established in 2021 and two bio-monitoring surveys were undertaken. The first on 11 June 2021 and the second on 19 January 2022. The results of these surveys will be reported on as part of the wider wellsite monitoring programme and have not been included in this report. Details of the surface water sites can be found in Table 4.

Table 4 Details of surface water sites included in the monitoring programme

Site code	Eastings	Northings	Distance from wellsite (m)
PRH000046	1713407	5682306	10m upstream of Turangi-B wellsite discharge
PRH000047	1713402	5682342	25m downstream of Turangi-B wellsite discharge
PRH000048	1713383	5682392	120m downstream of Turangi-B wellsite discharge

2. Results

2.1 Physicochemical sampling

2.1.1 Groundwater

Hydraulic fracturing activities commenced at the Turangi-B wellsite on 23 July 2021 and continued until 8 June 2023. A pre-fracturing baseline sample was collected on 26 February 2021. Post fracturing samples were collected at various intervals following commencement of the activities which including hydraulic fracturing in five wells and spanned 23 months. Interim samples were collected on 9 July 2021, 23 December 2021, 14 June 2022, 14 April 2023, 15 August 2023, and 27 September 2023. A post fracturing sample was collected on 18 April 2024.

Methane concentrations $> 1\text{g/m}^3$ were reported in all of the samples both pre and post-hydraulic fracturing activities and can occur as a result of biogenic processes in sulphate depleted groundwater systems. To determine whether the source of the methane was biogenic or thermogenic, the majority of samples were sent to Geological and Nuclear Sciences (GNS) for carbon 13 isotope analysis. The presence of carbon 13 isotopes concentrations at less than -50‰ indicate a thermogenic deep gas source and concentrations greater than -50‰ a shallow biogenic gas source. Carbon 13 concentrations ranged between -40.1 to 72.1‰ indicating a mixed biogenic/thermogenic source of methane at the site.

Overall, samples demonstrate relatively narrow ranges in analyte concentrations over time. The subtle variation in analyte concentrations are a result of natural seasonal fluctuation and sampling variability. The results of the laboratory analysis indicate there have been no significant changes in groundwater composition over the period monitored.

A summary of the results for groundwater samples taken in relation to the hydraulic fracturing activities compared to baseline is included in Table 5. The certificates of analysis for the review period are included in Appendix III.

Table 5 Results of groundwater sampling carried out in relation to the Turangi-B fracturing events

Sample date	unit	25/02/21	09/07/2021	23/12/2021	14/06/2022	14/04/2023	15/08/2023	27/09/2023	18/04/2024
Sample time	-	11:05	11:20	09:42	12:47	12:30	10:38	10:20	11:45
Sample id. TRC	-	TRC210881	TRC212297	TRC214610	TRC226761	TRC2311843	TRC2313713	TRC2314267	TRC2418074
pH	pH	7.4	6.9	7.1	7.1	7.4	7.4	7.0	7.0
Temperature	°C	17.1	15.0	17.0	15.0	16.0	14.9	14.8	16.0
Total alkalinity	g/m ³ CaCO ₃	167	159	149	141	164	159	159	171
Bicarbonate	g/m ³ HCO ₃	200	194	182	172	200	194	194	210
Total hardness	g/m ³ CaCO ₃	108	125	112	105	120	127	133	127
Electrical conductivity	µS/cm	360	361	327	312	353	341	356	362
Total dissolved solids	g/m ³	220	240	240	260	240	240	250	270
Dissolved calcium	g/m ³	24	30	26	24	27	30	31	29
Chloride	g/m ³	16.3	16.4	17.1	16.6	17.1	15.5	16.6	16.7
Dissolved magnesium	g/m ³	12.0	12.3	11.4	10.8	12.5	12.7	0.44	13.4
Dissolved potassium	g/m ³	7	5.2	5.5	4.2	6.0	5.1	5.1	6.2
Dissolved sodium	g/m ³	28	21	21	18.8	27	21	22	26
Nitrite	g/m ³ N	0.004	<0.02	<0.02	< 0.02	0.006	0.005	0.005	0.005
Nitrate	g/m ³ N	0.012	<0.02	< 0.02	< 0.02	0.006	0.014	< 0.002	<0.002
Nitrate & nitrite	g/m ³ N	0.016	<0.02	<0.02	< 0.02	0.011	0.019	0.005	0.003
Sulphate	g/m ³	<0.5	1	<0.5	< 0.5	< 0.5	<0.5	< 0.5	< 0.5
Dissolved barium	g/m ³	0.033	0.064	0.047	0.051	0.048	0.056	0.065	0.048
Bromide	g/m ³	0.06	0.09	0.09	0.07	0.10	0.08	0.08	0.07
Dissolved copper	g/m ³	< 0.0005	< 0.0005	< 0.0005	< 0.0005	< 0.0005	< 0.0005	< 0.0005	< 0.005
Dissolved iron	g/m ³	4.5	10.8	8.3	9.4	8.1	9.6	12.1	8.1
Dissolved manganese	g/m ³	0.23	0.48	0.37	0.38	0.31	0.40	0.44	0.31
Dissolved mercury	g/m ³	< 0.00008	< 0.00008	< 0.00008	< 0.00008	< 0.00008	< 0.00008	< 0.00008	< 0.00008
Dissolved Nickel	g/m ³	< 0.0005	0.0005	< 0.0005	< 0.0006	< 0.0005	< 0.0005	< 0.0005	< 0.0005
Dissolved zinc	g/m ³	0.0052	0.0044	0.0113	0.0116	<0.0010	0.0022	0.0035	0.0093

Sample date	unit	25/02/21	09/07/2021	23/12/2021	14/06/2022	14/04/2023	15/08/2023	27/09/2023	18/04/2024
Sample time	-	11:05	11:20	09:42	12:47	12:30	10:38	10:20	11:45
Sample id. TRC	-	TRC210881	TRC212297	TRC214610	TRC226761	TRC2311843	TRC2313713	TRC2314267	TRC2418074
Ethylene glycol	g/m ³	< 4	< 4	< 4	< 4	< 4	< 4	< 4	< 4
Propylene glycol	g/m ³	< 4	< 4	< 4	< 4	< 4	< 4	< 4	< 4
Methanol	g/m ³	< 4	< 2	< 2	< 2	< 2	< 2	< 2	< 2
Benzene	g/m ³	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	<0.0010
Toluene	g/m ³	<0.0010	< 0.0010	< 0.0010	0.0014	< 0.0010	< 0.0010	< 0.0010	<0.0010
Ethylbenzene	g/m ³	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	<0.0010
m-Xylene	g/m ³	< 0.002	< 0.002	< 0.002	< 0.002	< 0.002	< 0.002	< 0.002	<0.002
o-Xylene	g/m ³	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	< 0.0010	<0.0010
Formaldehyde	g/m ³	< 0.02	0.02	< 0.02	< 0.02	< 0.02	<0.02	< 0.02	0.02
Ethane	g/m ³	< 0.003	< 0.003	< 0.003	< 0.003	< 0.003	< 0.003	< 0.003	< 1
Ethylene	g/m ³	< 0.004	< 0.004	< 0.004	< 0.004	< 0.004	< 0.004	< 0.004	< 1
Methane	g/m ³	8.3	14.2	11.2	11.7	12.3	14.5	15.7	8.7
C7-C9 hydrocarbons	g/m ³	< 0.10	< 0.10	< 0.10	< 0.10	< 0.10	< 0.10	< 0.10	< 0.10
C10-C14 hydrocarbons	g/m ³	< 0.2	< 0.2	< 0.2	< 0.2	< 0.2	< 0.2	< 0.2	< 0.2
C15-C36 hydrocarbons	g/m ³	< 0.4	< 0.4	< 0.4	< 0.4	< 0.4	< 0.4	< 0.4	< 0.4
Total hydrocarbons	g/m ³	< 0.7	< 0.7	< 0.7	< 0.7	< 0.7	< 0.7	< 0.7	< 0.7
δ13C value	‰	-60.4	-69.6	-72.1	-40.1	-69.7	-70.3	-70.5	-

2.2 Consent holder submitted data

The conclusions from the Turangi-B post fracturing discharge reports are summarised as follows:

2.2.1 Turangi-11 post fracturing discharge report

- A total of two zones were fractured over the period 23 July 2021 to 17 November 2022 at mid-point depths between 3,404.8 to 3,414m TVDss.
- A total of 2,740bbls (435.6m³) of liquid was discharged across the two fractured units. The total proppant weight was 64.8 tonnes (142,919lbs).
- The majority of fluid injected was returned from the well over the flow-back period with any remaining fluid expected to be returned during subsequent operations.
- A total of 64.8 tonnes (142,919lbs) of proppant was estimated to have remained within the formation following flow-back.
- No screen outs occurred during hydraulic fracturing of the Turangi-11 well.
- All return fluid from the Turangi-11 fracturing operations were disposed of at the Company's Kaimiro-G wellsite under the Company's deep well injection consent.
- Pressure testing was undertaken of all surface equipment, including flow lines and the wellhead, prior to injection.
- There was no escape of fluids during hydraulic fracturing operations.

2.2.2 Turangi-14 post fracturing discharge report

- A total of two zones were fractured over the period 2 September to 8 September 2021 at mid-point depths between 3,954 to 4,074m TVDss.
- A total of 3,105bbls (493.6m³) of liquid was discharged across the two fractured units. The total proppant weight was 88.6 tonnes (195,384lbs).
- All fluid injected was returned from the well over the flow-back period.
- A total of 88.6 tonnes (195,384lbs) of proppant was estimated to have remained within the formation following flow-back.
- No screen outs occurred during hydraulic fracturing of the Turangi-14 well.
- All return fluid from the Turangi-14 fracturing operations were disposed of at the Company's Kaimiro-G wellsite under the Company's deep well injection consent.
- Pressure testing was undertaken of all surface equipment, including flow lines and the wellhead, prior to injection.
- There was no escape of fluids during hydraulic fracturing operations.

2.2.3 Turangi-16 post fracturing discharge report

- A total of seven zones were fractured over the period 24 March 2022 to 19 May 2022 at mid-point depths between 3,415 to 4,538m TVDss.
- A total of 10,509bbls (1,670m³) of liquid was discharged across the seven fractured units. The total proppant weight was 265.5 tonnes (585,447lbs).
- The majority of fluid injected was returned from the well over the flow-back period with any remaining fluid expected to be returned during subsequent operations.
- A total of 257.3 tonnes (567,303lbs) of proppant was estimated to have remained within the formation following flow-back.

- Treatments 1 and 5 screened out during hydraulic fracturing of the Turangi-16 well resulting in under-displacement of some proppant in the wellbore. This was all recovered during coiled tubing and has no implications in compliance with conditions 1 and 5 of the consent. No further screenouts occurred during the stimulation treatments.
- All return fluid from the Turangi-16 fracturing operations were disposed of at the Company's Kaimiro-G wellsite under the Company's deep well injection consent.
- Pressure testing was undertaken of all surface equipment, including flow lines and the wellhead, prior to injection.
- There was no escape of fluids during hydraulic fracturing operations.

2.2.4 Turangi-18 post fracturing discharge report

- A total of six zones were fractured over the period 5 December 2022 to 1 February 2023 at mid-point depths between 3,421 to 4,036m TVDss.
- A total of 9,015bbls (1,433.2m³) of liquid was discharged across the six fractured units. The total proppant weight was 214.4 tonnes (472,721lbs).
- The majority of fluid injected was returned from the well over the flow-back period with any remaining fluid expected to be returned during subsequent operations.
- A total of 213.6 tonnes (470,957lbs) of proppant was estimated to have remained within the formation following flow-back.
- Treatment 6 screened out during hydraulic fracturing of the Turangi-18 well resulting in under-displacement of some proppant in the wellbore. This was all recovered with coiled tubing and has no implications in compliance with conditions 1 and 5 of the consent. No further screen outs occurred during the stimulation treatments.
- All return fluid from the Turangi-18 fracturing operations were disposed of at the Company's Kaimiro-G wellsite under the Company's deep well injection consent.
- Pressure testing was undertaken of all surface equipment, including flow lines and the wellhead, prior to injection.
- There was no escape of fluids during hydraulic fracturing operations.

2.2.5 Turangi-19 post fracturing discharge report

- A total of six zones were fractured over the period 28 April 2023 to 8 June 2023 at mid-point depths between 3,419.9 to 4,084.4m TVDss.
- A total of 11,616 bbls (1,846.7m³) of liquid was discharged across the six fractured units. The total proppant weight was 239.9 tonnes (528,920lbs).
- The majority of fluid injected was returned from the well over the flow-back period with any remaining fluid expected to be returned during subsequent operations.
- A total of 239.9 tonnes (528,920lbs) of proppant was estimated to have remained within the formation following flow-back.
- There were no screen outs during hydraulic fracturing of the Turangi-19 well.
- All return fluid from the Turangi-19 fracturing operations were disposed of at the Company's Kaimiro-G wellsite under the Company's deep well injection consent.
- Pressure testing was undertaken of all surface equipment, including flow lines and the wellhead, prior to injection.
- There was no escape of fluids during hydraulic fracturing operations.

2.2.6 Hydraulic fracturing and return fluids

The results of the analyses carried out on samples of the hydraulic fracturing fluid used in the stimulation of the Turangi-11, Turangi-14, Turangi-16, Turangi-18 and Turangi-19 wells are shown below in Table 6. The certificates of analysis are included in Appendix IV.

The results of the analyses carried out on the return fluid samples obtained following the hydraulic fracturing of the Turangi-11, Turangi-14, Turangi-16, Turangi-18 and Turangi-19 wells are summarised below in Table 7. The certificates of analysis are included in Appendix IV. The results demonstrate the variability of groundwater composition and hydrocarbon concentrations during flow-back. The relatively high levels of chloride, sodium and hydrocarbons in each sample indicate that the composite samples prepared contained a greater proportion of reservoir fluids than hydraulic fracturing fluids introduced during the fracturing activities, which are comprised predominantly of freshwater.

Table 6 Results of hydraulic fracturing fluid sampling

Well	Unit	Turangi-11		Turangi-14		Turangi-16		Turangi-18		Turangi-19	
Parameter	Range	Min	Max	Min	Max	Min	Max	Min	Max	Min	Max
Ethylene glycol*	g/m ³	< 2	720	< 2	560	460	1,080	71	820	77	860
Propylene Glycol*	g/m ³	< 2	< 2	< 2	< 2	< 2	< 4	< 2	< 2	< 2	< 400
Methanol*	g/m ³	< 2	< 2	< 2	< 2	< 2	< 2	< 2	2	< 2	< 110
Benzene	g/m ³	0.0015	0.0031	0.008	0.124	< 0.001	0.0096	0.002	0.0035	< 0.0010	0.0031
Toluene	g/m ³	0.0027	0.0183	0.018	0.056	< 0.001	0.0174	0.0087	0.02	0.0021	0.0038
Ethylbenzene	g/m ³	< 0.001	0.0023	< 0.008	0.0056	< 0.001	0.0015	0.0014	0.0027	< 0.0010	< 0.0010
0.003	g/m ³	0.017	< 0.02	< 0.02	0.043	< 0.002	0.007	0.009	0.018	0.002	0.003
o-Xylene	g/m ³	< 0.001	0.0064	< 0.01	0.0146	< 0.001	0.0015	0.0047	0.0052	0.0011	0.0014
C7-C9	g/m ³	0.8	< 0.5	< 0.5	5	< 0.15	< 0.4	< 0.2	< 0.5	< 0.5	< 0.5
C10-C14	g/m ³	< 1.0	3,500	< 1	4,100	< 0.4	< 1.0	< 0.4	< 1	< 1.0	< 1.0
C15-C36	g/m ³	3	183	< 2	350	< 0.8	15	1.5	160	< 2	3
Total hydrocarbons	g/m ³	< 4	3,700	< 4	4,400	< 1.4	16	1.5	160	< 4	< 4

Note * Depending on the viscosity of the sample received at the laboratory, samples may require dilution prior to analysis which results in higher detection limits.

Table 7 Results of hydraulic fracturing return fluid sampling

Well	Unit	Turangi-11		Turangi-14		Turangi-16		Turangi-18		Turangi-19	
Parameter	Range	Min	Max	Min	Max	Min	Max	Min	Max	Min	Max
pH	pH	6.9	8.2	6.9	7.1	5.9	7.3	6.6	6.8	6.7	7.7
Total Alkalinity	g/m ³ as CaCO ₃	1,440	1,460	700	930	102	1,670	450	1,330	580	2,100
Total Hardness	g/m ³ as CaCO ₃	128	280	230	440	89	430	131	320	96	400
Electrical Conductivity	mS/m	1,878	6,040	1,471	1,856	90.4	1,839	775	1,798	867	1,756
Total Dissolved Solids	g/m ³	5,400	12,600	10,900	12,200	3,200	15,300	7,000	13,400	7,400	12,400
Dissolved Barium	g/m ³	2.3	40	32	41	0.106	43	7.4	54	2.4	25
Dissolved Bromine	g/m ³	5.5	17.4	16.6	18.4	<0.5	19.4	5.3	24	7.8	19.7
Dissolved Calcium	g/m ³	42	89	78	150	24	152	43	109	29	133
Dissolved Copper	g/m ³	< 0.005	0.005	0.027	0.031	0.007	0.092	0.009	0.34	0.005	0.56

Well	Unit	Turangi-11		Turangi-14		Turangi-16		Turangi-18		Turangi-19	
Parameter	Range	Min	Max	Min	Max	Min	Max	Min	Max	Min	Max
Dissolved Iron	g/m ³	5.2	10.1	1.94	2.7	2.5	6.0	1.66	7.9	0.83	9.4
Dissolved Magnesium	g/m ³	6	13	9	16	7	14	6	16	5	18
Dissolved Manganese	g/m ³	3.3	4.9	3.3	5.5	0.52	1.8	0.44	2.4	0.52	2.4
Total Nickel	g/m ³	0.22	0.41	0.125	0.198	< 0.032	1.06	0.07	0.39	0.04	1.17
Total Potassium	g/m ³	146	185	194	240	13	141	64	330	61	158
Total Sodium	g/m ³	1,250	4,000	2,800	3,900	63	3,800	1,760	3,900	1,850	3,600
Total Sulphur	g/m ³	7	11	13	14	7.6	16.5	8	< 60	10	< 60
Total Zinc	g/m ³	0.036	0.153	0.42	0.142	0.068	0.56	0.08	0.76	0.042	1.83
Chloride	g/m ³	1,180	5,900	4,400	6,100	240	5,800	1,180	5,900	1,740	6,000
Nitrite	g/m ³ N	< 0.010	< 0.05	0.64	0.67	< 0.0010	< 0.1	< 0.10	< 0.10	< 0.10	< 0.10
Nitrate	g/m ³ N	< 0.010	0.05	< 0.010	0.024	< 0.0010	< 0.1	< 0.10	0.14	< 0.10	< 0.10
Nitrate+Nitrite	g/m ³ N	0.08	<0.10	0.063	0.091	< 0.05	< 0.1	< 0.5	0.6	< 0.5	< 0.5
Sulphate	g/m ³	21	34	40	42	23	49	24	< 160	30	< 160
Ethylene glycol	g/m ³	< 20	120	153	172	< 2	220	< 20	55	< 20	39
Propylene glycol	g/m ³	< 2	< 2	< 20	< 20	< 2	52	< 20	< 20	< 20	< 20
Methanol	g/m ³	< 2	400	< 20	410	< 2	< 2	< 20	36	< 20	< 110
Benzene	g/m ³	10	17.9	63	171	3.5	660	9.6	17.3	15.8	44
Toluene	g/m ³	6.2	28	100	260	1.09	1,630	7.0	44	14.9	88
Ethylbenzene	g/m ³	0.23	2.6	22	29	0.025	330	0.4	4.3	1.02	44
m&p-Xylene	g/m ³	1.21	16.7	135	172	0.115	1,220	2.2	30	5.9	18.2
o-Xylene	g/m ³	0.5	5.3	39	51	0.073	570	0.8	9.3	2.1	23
Formaldehyde	g/m ³	< 0.15	< 0.15	< 0.15	<0.15	< 0.15	1.7	< 0.15	4	< 0.15	< 1.5
C7-C9	g/m ³	16	260	3,600	3,800	4.0	1,450	17	5,700	94	6,900
C10-C14	g/m ³	104	580	5,700	6,200	6.1	1,260	45	9,300	240	9,600
C15-C3	g/m ³	52	400	4,200	5,100	11.7	660	104	14,400	330	12,200
Total hydrocarbons	g/m ³	173	1,240	13,700	14,900	22	3,40077	166	29,000	690	21,000

Note * Depending on the viscosity of the sample received at the laboratory, samples may require dilution prior to analysis which results in higher detection limit.

2.3 Incidents, investigations, and interventions

The monitoring programme for the year was based on what was considered to be an appropriate level of monitoring, review of data, and liaison with the Company. During the year matters may arise which require additional activity by the Council, for example provision of advice and information, or investigation of potential or actual causes of non-compliance or failure to maintain good practices. A pro-active approach, that in the first instance avoids issues occurring, is favoured.

For all significant compliance issues, as well as complaints from the public, the Council maintains a database record. The record includes events where the individual/organisation concerned has itself notified the Council. Details of any investigation and corrective action taken are recorded for non-compliant events.

Complaints may be alleged to be associated with a particular site. If there is potentially an issue of legal liability, the Council must be able to prove by investigation that the identified individual/organisation is indeed the source of the incident (or that the allegation cannot be proven).

In the 2021-2023 period, the Council was not required to undertake significant additional investigations and interventions, or record incidents, in association with the Company's conditions in resource consents or provisions in Regional Plans.

3. Discussion

3.1 Environmental effects of exercise of consent

Five wells (Turangi-11, Turangi-14, Turangi-16, Turangi-18 and Turangi-19) were stimulated by hydraulic fracturing at the Turangi-B wellsite during the period 23 July 2021 to 8 June 2023.

The monitoring programme carried out by the Council in relation to the fracturing events undertaken included pre and post fracturing sampling at one groundwater monitoring site in the vicinity of the Turangi-B wellsite. The results of post fracturing groundwater sampling carried out generally showed only very minor variations in water composition in comparison to baseline results. The minor variations in analytes are a result of natural variations in water composition.

There was no surface water monitoring undertaken in relation to hydraulic fracturing activities at the wellsite.

In summary, the monitoring carried out by the Council during the period being reported indicated that the hydraulic fracturing activities undertaken by the Company at the Turangi-B wellsite have had no significant adverse effects on local groundwater or surface water resources.

3.2 Evaluation of performance

A tabular summary of the consent holder's compliance record for the year under review is set out in Table 8.

Table 8 Summary of performance for consent 7952-2

Purpose: To discharge water based hydraulic fracturing fluids into land at depths greater than 3,410 metres true vertical depth subsea (TVDss) beneath the Turangi-B wellsite		
Condition requirement	Means of monitoring during period under review	Compliance achieved?
1. Any discharge shall occur below 3,410m TVDss	Assessment of consent holder submitted data	Yes
2. No discharge shall occur after 1 June 2028	Assessment of consent holder submitted data	N/A
3. Monitoring and reporting of seismic events within 5km of any discharge location	Notification and post fracturing report	N/A
4. Actions to be taken following the occurrence of any event described in condition 3	Notification under condition 3	N/A
5. Exercise of consent shall not result in any contaminants reaching any useable freshwater	Results of groundwater monitoring	Yes
6. Consent holder shall undertake sampling programme	Development and certification of a monitoring programme	Yes
7. If no suitable bores exist within 500m of the wellsite, a monitoring bore may need to be installed	Inspection of bores	Yes
8. Sampling programme shall follow recognised field procedures and be analysed for a specified range of chemical parameters	Development and certification of a monitoring programme and assessment of results	Yes
9. All sampling to be carried out in accordance with a certified Sampling and Analysis Plan	Development and certification of a Sampling and Analysis Plan	Yes

Purpose: To discharge water based hydraulic fracturing fluids into land at depths greater than 3,410 metres true vertical depth subsea (TVDss) beneath the Turangi-B wellsite		
Condition requirement	Means of monitoring during period under review	Compliance achieved?
10. Well and equipment pressure testing to be carried out prior to any hydraulic fracturing programme commencing	Assessment of consent holder submitted data	Yes
11. A pre-fracturing discharge report is to be provided to the Council 14 days prior to discharge	Pre-fracturing discharge report received	Yes
12. Consent holder shall notify the Council of hydraulic fracturing discharge	Notification received	Yes
13. A post fracturing discharge report is to be provided to the Council within 90 days of any commencement	Post fracturing discharge report received	Yes
14. For programs including multiple hydraulic fracturing discharges, more than one 'Post-fracturing discharge report' may be required	Reports received	Yes
15. Reports in condition 11 and 13 emailed to consents@trc.govt.nz commencement of any hydraulic fracturing	Reports received via email	Yes
16. The consent holder shall provide access to a location where samples of hydraulic fracturing fluids and return fluids can be obtained by the Council officers	Access provided	Yes
17. Consent holder to adopt best practicable option at all times	Site inspections, sampling and assessment of consent holder submitted data	Yes
18. Fracture fluid comprised of no less than 95% water and proppant by volume	Assessment of consent holder submitted data and sampling of fracturing fluid	Yes
19. Lapse clause	Consent exercised	Yes
20. Review condition	N/A	N/A
Overall assessment of environmental performance and compliance in respect of this consent		High
Overall assessment of administrative performance and compliance in respect of this consent		High

N/A=not applicable

Table 9 Evaluation of environmental performance over time)

Year	Consent numbers	High	Good	Improvement req	Poor
2019-2022	7952-2	1	-	-	-
2021-2023	7952-2	1	-	-	-

During the monitoring period, the Company demonstrated a high level of environmental and high level of administrative performance with the resource consent as defined in Appendix II.

3.3 Recommendations from the 2019-2021 Report

In the 2019-2021 report, it was recommended:

1. THAT in the first instance, the range of monitoring carried out during the reporting period in relation to the Company's hydraulic fracturing activities be replicated for any future fracturing events at the Turangi-B wellsite.

2. THAT should there be issues with environmental or administrative performance in future periods, monitoring may be adjusted to reflect any additional investigation or intervention as found necessary.
3. THAT the option for a review of resource consents in June 2024, as set out in condition 20 of the consent not be exercised.

Recommendation 1 was implemented, recommendation 2 was not required and recommendation 3 was accepted by Council.

3.4 Alterations to monitoring programmes for future hydraulic fracturing activities

In designing and implementing the monitoring programmes for air/water discharges in the region, the Council has taken into account:

- the extent of information already made available through monitoring or other means to date;
- its relevance under the RMA;
- the Council's obligations to monitor consented activities and their effects under the RMA;
- the record of administrative and environmental performances of the consent holder; and
- reporting to the regional community.

The Council also takes into account the scope of assessments required at the time of renewal of permits, and the need to maintain a sound understanding of industrial processes within Taranaki exercising resource consents.

It is proposed that the range of monitoring carried out in relation to the hydraulic fracturing activities undertaken by the Company be replicated for any future fracturing events at the Turangi-B wellsite.

A recommendation to this effect is included in Section 4 of this report.

It should be noted that the proposed programme represents a reasonable and risk-based level of monitoring for the site in question. The Council reserves the right to subsequently adjust the programme from that initially prepared, should the need arise if potential or actual non-compliance is determined at any time during future monitoring periods.

4. Recommendations

1. THAT in the first instance, the range of monitoring carried out during the reporting period in relation to the Company's hydraulic fracturing activities be replicated for any future fracturing events at the Turangi-B wellsite.
2. THAT should there be issues with environmental or administrative performance in future periods, monitoring may be adjusted to reflect any additional investigation or intervention as found necessary.

Glossary of common terms and abbreviations

The following abbreviations and terms may be used within this report:

Biomonitoring	Assessing the health of the environment using aquatic organisms.
bbls	Barrel. Unit of measure used in the oil and gas industry (equivalent to approximately 159L).
Conductivity	An indication of the level of dissolved salts in a sample, usually measured at 25°C and expressed in $\mu\text{S}/\text{cm}$.
DO	Dissolved oxygen.
E.coli	Escherichia coli, an indicator of the possible presence of faecal material and pathological micro-organisms. Usually expressed as colony forming units per 100 millilitre sample.
EPT	Ephemeroptera (mayfly), Plecoptera (stonefly) and Trichoptera (caddisfly) which are macroinvertebrates sensitive to pollution.
Fresh	Elevated flow in a stream, such as after heavy rainfall.
g/m^3	Grams per cubic metre, and equivalent to milligrams per litre (mg/L). In water, this is also equivalent to parts per million (ppm), but the same does not apply to gaseous mixtures.
Incident	An event that is alleged or is found to have occurred that may have actual or potential environmental consequences or may involve non-compliance with a consent or rule in a regional plan. Registration of an incident by the Council does not automatically mean such an outcome had actually occurred.
Intervention	Action/s taken by Council to instruct or direct actions be taken to avoid or reduce the likelihood of an incident occurring.
Investigation	Action taken by Council to establish the circumstances/events surrounding an incident including any allegations of an incident.
L/s	Litres per second.
Macroinvertebrate	An invertebrate that is large enough to be seen without the use of a microscope.
masl	Metres above sea level.
MCI	Macroinvertebrate community index; a numerical indication of the state of biological life in a stream that takes into account the sensitivity of the taxa present to organic pollution in stony habitats.
mS/m	Millisiemens per metre.
m^3	Cubic metre (1,000L).
NZTM	New Zealand Transverse Mercator coordinates.
pH	A numerical system for measuring acidity in solutions, with 7 as neutral. Numbers lower than 7 are increasingly acidic and higher than 7 are increasingly alkaline.
Physicochemical	Measurement of both physical properties (e.g. temperature, clarity, density) and chemical determinants (e.g. metals and nutrients) to characterise the state of an environment.
Resource consent	Refer Section 87 of the RMA. Resource consents include land use consents (refer Sections 9 and 13 of the RMA), coastal permits (Sections 12, 14 and 15), water permits (Section 14) and discharge permits (Section 15).
RMA	Resource Management Act 1991 and including all subsequent amendments.

Screen Out	A condition that occurs when the solids carried in a treatment fluid, such as proppant in a fracture fluid, create a bridge across the perforations or similar restricted flow area. This creates a sudden and significant restriction to fluid flow that causes a rapid rise in pump pressure.
SQMCI	Semi quantitative macroinvertebrate community index.
TVDss	True vertical depth sub-sea.
$\mu\text{S/cm}$	Microsiemens per centimetre.
Workover	The repair or stimulation of an existing production well for the purpose of restoring, prolonging or enhancing the production of hydrocarbons.

For further information on analytical methods, contact an Environment Quality Manager.

Bibliography and references

Baker Hughes at <http://blogs.bakerhughes.com/reservoir/2012/02/20/hydraulic-fracturing-an-environmentally-responsible-technology-for-ensuring-our-energy-future-part-iii-of-iii>

Geology.Com at <http://geology.com/energy/hydraulic-fracturing-fluids/>

Ministry for the Environment. 2018. Guidelines for compliance monitoring and enforcement under the Resource Management Act 1991. Wellington: Ministry for the Environment

Greymouth Petroleum Ltd (2021): Turangi-B Hydraulic Fracturing Monitoring Programme Report 2019-2021 Technical Report 22-97. Frodo number #3133741

Greymouth Petroleum Ltd (2019): Turangi-B water quality monitoring programme. Frodo number #2330433

Greymouth Petroleum Ltd (2021): Turangi-11 Pre-Stimulation Discharge Report, January 2021. Frodo number #2700756

Greymouth Petroleum Ltd (2021): Turangi-14 Pre-Stimulation Discharge Report, July 2021. Frodo number #2830160

Greymouth Petroleum Ltd (2021): Turangi-16 Pre-Stimulation Discharge Report, November 2021. Frodo number #2957945

Greymouth Petroleum Ltd (2022): Turangi-18 Pre-Stimulation Discharge Report, October 2022. Frodo number #3120609

Greymouth Petroleum Ltd (2023): Turangi-19 Pre-Stimulation Discharge Report, February 2023. Frodo number #3152152

Greymouth Petroleum Ltd (2022): Turangi-14 Post-Stimulation Discharge Report, November 2022. Frodo number #2997826

Greymouth Petroleum Ltd (2022): Turangi-16 Post-Stimulation Discharge Report, June 2022. Frodo number #2572456

Greymouth Petroleum Ltd (2023): Turangi-18 Post-Stimulation Discharge Report, February 2023. Frodo number #3148241

Greymouth Petroleum Ltd (2023): Turangi-11 Post-Stimulation Discharge Report, February 2023. Frodo number #3147107

Greymouth Petroleum Ltd (2023): Turangi-19 Post-Stimulation Discharge Report, July 2023. Frodo number #3219567

Appendix I

Resource consent held by Greymouth Petroleum Turangi Ltd

(For a copy of the signed resource consent
please contact the TRC Consents department)

Water abstraction permits

Section 14 of the RMA stipulates that no person may take, use, dam or divert any water, unless the activity is expressly allowed for by a resource consent or a rule in a regional plan, or it falls within some particular categories set out in Section 14. Permits authorising the abstraction of water are issued by the Council under Section 87(d) of the RMA.

Water discharge permits

Section 15(1)(a) of the RMA stipulates that no person may discharge any contaminant into water, unless the activity is expressly allowed for by a resource consent or a rule in a regional plan, or by national regulations. Permits authorising discharges to water are issued by the Council under Section 87(e) of the RMA.

Air discharge permits

Section 15(1)(c) of the RMA stipulates that no person may discharge any contaminant from any industrial or trade premises into air, unless the activity is expressly allowed for by a resource consent, a rule in a regional plan, or by national regulations. Permits authorising discharges to air are issued by the Council under Section 87(e) of the RMA.

Discharges of wastes to land

Sections 15(1)(b) and (d) of the RMA stipulate that no person may discharge any contaminant onto land if it may then enter water, or from any industrial or trade premises onto land under any circumstances, unless the activity is expressly allowed for by a resource consent, a rule in a regional plan, or by national regulations. Permits authorising the discharge of wastes to land are issued by the Council under Section 87(e) of the RMA.

Land use permits

Section 13(1)(a) of the RMA stipulates that no person may in relation to the bed of any lake or river use, erect, reconstruct, place, alter, extend, remove, or demolish any structure or part of any structure in, on, under, or over the bed, unless the activity is expressly allowed for by a resource consent, a rule in a regional plan, or by national regulations. Land use permits are issued by the Council under Section 87(a) of the RMA.

Coastal permits

Section 12(1)(b) of the RMA stipulates that no person may erect, reconstruct, place, alter, extend, remove, or demolish any structure that is fixed in, on, under, or over any foreshore or seabed, unless the activity is expressly allowed for by a resource consent, a rule in a regional plan, or by national regulations. Coastal permits are issued by the Council under Section 87(c) of the RMA.

Discharge Permit
Pursuant to the Resource Management Act 1991
a resource consent is hereby granted by the
Taranaki Regional Council

Name of
Consent Holder: Greymouth Petroleum Turangi Limited
PO Box 3394
Fitzroy
New Plymouth 4341

Decision Date: 9 June 2016

Commencement Date: 9 June 2016

Conditions of Consent

Consent Granted: To discharge water based hydraulic fracturing fluids into land at depths greater than 3,410 mTVDss beneath the Turangi-B wellsite

Expiry Date: 1 June 2033

Review Date(s): June annually and in accordance with special condition 20

Site Location: Turangi-B wellsite, 42 Turangi Road Upper, Tikorangi
(Property owner: RJ Topless)

Grid Reference (NZTM) 1713599E-5682493N

Catchment: Parahaki

*For General, Standard and Special conditions
pertaining to this consent please see reverse side of this document*

Page 1 of 6

General condition

- a. The consent holder shall pay to the Taranaki Regional Council all the administration, monitoring and supervision costs of this consent, fixed in accordance with section 36 of the Resource Management Act 1991.

Special conditions

1. The discharge point shall be deeper than 3,410 mTVDss.

Note: mTVDss = metres true vertical depth subsea, i.e., the true vertical depth in metres below mean sea level
2. There shall be no discharge of hydraulic fracturing fluids after 1 June 2028.
3. If the GeoNet seismic monitoring network records a seismic event higher than a Modified Mercalli intensity of magnitude 3.0 within 5 km of the geographical position (in 3 dimensions) of any hydraulic fracturing discharge, then:
 - (a) if a hydraulic fracturing discharge is currently being undertaken it shall cease immediately and not recommence; or
 - (b) if a hydraulic fracturing discharge has occurred within the previous 72 hours no further hydraulic fracturing discharges shall occur.
4. Following the occurrence of any seismic event described in special condition 3 the consent holder shall investigate and report to the Chief Executive, Taranaki Regional Council on the likelihood of the seismic event being induced by the exercise of this consent. Hydraulic fracturing discharges may only then continue once the Chief Executive, Taranaki Regional Council has considered the report and concluded that the environmental risk of recommencing hydraulic fracturing is acceptable and has advised the consent holder accordingly.
5. The consent holder shall ensure that the exercise of this consent does not result in contaminants reaching any useable fresh water (groundwater or surface water). Usable fresh groundwater is defined as any groundwater having a Total Dissolved Solids concentration of less than 1,000 mg/l.
6. The consent holder shall undertake a programme of sampling and testing that monitors the effects of the exercise of this consent on fresh water resources to assess compliance with condition 5 (the 'Monitoring Programme'). The Monitoring Programme shall be certified by the Chief Executive, Taranaki Regional Council ('the Chief Executive'), before this consent is exercised, and shall include:
 - (a) the location of the discharge point(s);
 - (b) the location of sampling sites; and
 - (c) sampling frequency with reference to a hydraulic fracturing programme.

7. Depending on the suitability of existing bores within 500 metres of the wellsite for obtaining a representative groundwater sample, it may be necessary for the Monitoring Programme to include installation of, and sampling from, at least one monitoring bore. The bore(s) would be of a depth, location and design determined after consultation with the Chief Executive, Taranaki Regional Council and installed in accordance with NZS 4411:2001.
8. All water samples taken for monitoring purposes shall be taken in accordance with recognised field procedures and analysed for:
- (a) pH;
 - (b) conductivity;
 - (c) total dissolved solids;
 - (d) major ions (Ca, Mg, K, Na, total alkalinity, bromide, chloride, nitrate-nitrogen, and sulphate);
 - (e) trace metals (barium, copper, iron, manganese, nickel, and zinc);
 - (f) total petroleum hydrocarbons;
 - (g) formaldehyde;
 - (h) dissolved methane and ethane gas;
 - (i) methanol;
 - (j) glycols;
 - (k) benzene, toluene, ethylbenzene, and xylenes (BTEX); and
 - (l) carbon-13 composition of any dissolved methane gas discovered ($^{13}\text{C-CH}_4$).

Note: The samples required, under conditions of this consent could be taken and analysed by the Taranaki Regional Council or other contracted party on behalf of the consent holder.

9. All sampling and analysis shall be undertaken in accordance with a *Sampling and Analysis Plan*, which shall be submitted to the Chief Executive for review and certification before the first sampling is undertaken. The plan shall specify the use of standard protocols recognised to constitute good professional practice including quality control and assurance. An International Accreditation New Zealand (IANZ) accredited laboratory shall be used for all sample analysis. Results shall be provided to the Chief Executive within 30 days of sampling and shall include supporting quality control and assurance information. These results will be used to assess compliance with condition 5.

Note: The Sampling and Analysis Plan may be combined with the Monitoring Programme required by condition 6.

10. The consent holder shall undertake well and equipment pressure testing prior to any hydraulic fracture programme on a given well to ensure any discharge will not affect the integrity of the well and hydraulic fracturing equipment.

11. Any hydraulic fracture discharge shall only occur after the consent holder has provided a comprehensive 'Pre-fracturing Discharge Report' to the Chief Executive. The report shall be provided at least 14 days before the discharge is proposed to commence and shall detail the hydraulic fracturing programme proposed, including as a minimum:
- (a) the specific well in which each discharge is to occur, the intended fracture interval(s) ('fracture interval' is the discrete subsurface zone to receive a hydraulic fracture treatment), and the duration of the hydraulic fracturing programme;
 - (b) the number of discharges proposed and the geographical position (i.e. depth and lateral position) of each intended discharge point;
 - (c) the total volume of fracture fluid planned to be pumped down the well, including mini-fracture treatments, and their intended composition, including a list of all contaminants and Material Safety Data Sheets for all the chemicals to be used;
 - (d) the monitoring techniques to be used to determine the fate of discharged material;
 - (e) the results of the reviews required by condition 17;
 - (f) results of modelling showing an assessment of the likely extent and dimensions of the fractures that will be generated by the discharge;
 - (g) the preventative and mitigation measures to be in place to ensure the discharge does not cause adverse environmental effects and complies with condition 5;
 - (h) the extent and permeability characteristics of the geology above the discharge point to the surface;
 - (i) any identified faults within the modelled fracture length plus a margin of 50%, and the potential for adverse environmental effects due to the presence of the identified faults;
 - (j) the burst pressure of the well casing and the anticipated maximum well and discharge pressures and the duration of the pressures; and
 - (k) details of the disposal of any returned fluids, including any consents that are relied on to authorise the disposal; and
 - (l) details why the contaminants in the discharge and the monitoring techniques used comply with condition 17.

Note: For the avoidance of doubt, the information provided with a resource consent application would usually be sufficient to constitute a 'Pre-fracturing Discharge Report' for any imminent hydraulic fracturing discharge. The Pre-fracturing Discharge Report provided for any later discharge may refer to the resource consent application or earlier Pre-fracturing Discharge Reports noting any differences.

12. The consent holder shall notify the Taranaki Regional Council of the date that each discharge is intended to commence by emailing worknotification@trc.govt.nz. Notification also shall identify the 'Pre-fracturing Discharge Report', required by condition 11, which details the discharge and be given no less than 3 days before the intended discharge date. If any discharge occurs more than 30 days after the notification date, additional notification as specified in this condition is required.

13. Subject to condition 14, within 90 days of any commencement date as advised under condition 12, the consent holder shall submit a comprehensive 'Post-fracturing Discharge Report' to the Chief Executive. The report shall, as a minimum, contain:
 - (a) date and time of discharge;
 - (b) confirmation of the interval(s) where fracturing occurred for that programme, and the geographical position (i.e., depth and lateral position) of the discharge point for each fracture interval;
 - (c) the contaminant volumes and composition of fluid discharged into each fracture interval;
 - (d) the volume of return fluids from each fracture interval;
 - (e) an analysis for the constituents set out in conditions 8(a) to 8(k), in a return fluid sample taken within the first two hours of flow back, for each fracture interval if flowed back individually, or for the well if flowed back with all intervals comingled;
 - (f) an estimate of the volume of fluids (and proppant) remaining underground;
 - (g) the volume of water produced with the hydrocarbons (produced water) over the period beginning at the start of the hydraulic fracturing programme and ending 30 days after the programme is completed or after that period of production;
 - (h) an assessment of the extent and dimensions of the fractures that were generated by the discharge, based on modelling undertaken after the discharge has occurred and other diagnostic techniques, including production analysis, available to determine fracture length, height and containment;
 - (i) the results of pressure testing required by condition 10 and the top-hole pressure (psi), slurry rate (bpm), surface proppant concentration (lb/gal), bottom hole proppant concentration (lb/gal), and calculated bottom hole pressure (psi), as well as predicted values for each of these parameters; prior to, during and after each hydraulic fracture treatment;
 - (j) details of the disposal of any returned fluids, including any consents that are relied on to authorise the disposal;
 - (k) details of any incidents where hydraulic fracture fluid is unable to pass through the well perforations (screen outs) that occurred, their likely cause and implications for compliance with conditions 1 and 5; and
 - (l) results of the monitoring referred to in condition 11 (d); and
 - (m) an assessment of the effectiveness of the mitigation measures in place with specific reference to those described in the application for this consent.
14. On occasions, including for programs involving multiple hydraulic fracturing discharges, more than one 'Post-fracturing discharge report' may be required in order to meet the 90-day deadline from commencement required by condition 13. In these situations the consent holder shall submit an 'Interim Post-fracturing Discharge Report', which includes all the information that is available, to the Chief Executive within 90 days and a final Post-fracturing report as soon as practicable but within 90 days of the interim report.
15. The reports described in conditions 11 and 13 shall be emailed to consents@trc.govt.nz with a reference to the number of this consent.
16. The consent holder shall provide access to a location where the Taranaki Regional Council officers can obtain a sample of the hydraulic fracturing fluids and the return fluids.

17. The consent holder shall at all times adopt the best practicable option, as defined in section 2 of the Resource Management Act 1991, to prevent or minimize any actual or likely adverse effect of the activity on the environment by, as a minimum, ensuring that:
- (a) the discharge is contained within the fracture interval;
 - (b) regular reviews of monitoring techniques used to ensure the discharge does not cause adverse environmental effects are undertaken;
 - (c) regular reviews are undertaken of the preventative and mitigation measures adopted to ensure the discharge does not cause adverse environmental effects; and
 - (d) regular reviews of the chemicals used are undertaken with a view to reducing the toxicity of the chemicals used.
18. The fracture fluid shall be comprised of no less than 95% water and proppant by volume.
19. This consent shall lapse on 30 June 2021, unless the consent is given effect to before the end of that period or the Taranaki Regional Council fixes a longer period pursuant to section 125(1)(b) of the Resource Management Act 1991.
20. The Taranaki Regional Council may review any or all of the conditions of this consent by giving notice of review:
- a) during the month of June each year, and/or
 - b) within 30 days of receiving any investigation and report in accordance with special condition 4 above;

for the purposes of:

- (a) ensuring that the conditions are adequate to deal with any significant adverse effects on the environment arising from the exercise of this consent, which were either not foreseen at the time the application was considered or which it was not appropriate to deal with at the time; and/or
- (b) further specifying the best practicable option as required by condition 17; and/or
- (c) ensuring hydraulic fracturing operations appropriately take into account any best practice guidance published by a recognised industry association or environmental regulator.

Signed at Stratford on 9 June 2016

For and on behalf of
Taranaki Regional Council



A D McLay
Director - Resource Management

Appendix II

Categories used to evaluate environmental and administrative performance

Categories used to evaluate environmental and administrative performance

Environmental performance is concerned with actual or likely effects on the receiving environment from the activities during the monitoring year. Administrative performance is concerned with the Company's approach to demonstrating consent compliance in site operations and management including the timely provision of information to Council (such as contingency plans and water take data) in accordance with consent conditions.

Events that were beyond the control of the consent holder and unforeseeable (that is a defence under the provisions of the RMA can be established) may be excluded with regard to the performance rating applied. For example loss of data due to a flood destroying deployed field equipment.

The categories used by the Council for this monitoring period, and their interpretation, are as follows:

Environmental Performance

High: No or inconsequential (short-term duration, less than minor in severity) breaches of consent or regional plan parameters resulting from the activity; no adverse effects of significance noted or likely in the receiving environment. The Council did not record any verified unauthorised incidents involving environmental impacts and was not obliged to issue any abatement notices or infringement notices in relation to such impacts.

Good: Likely or actual adverse effects of activities on the receiving environment were negligible or minor at most. There were some such issues noted during monitoring, from self-reports, or during investigations of incidents reported to the Council by a third party but these items were not critical, and follow-up inspections showed they have been dealt with. These minor issues were resolved positively, co-operatively, and quickly. The Council was not obliged to issue any abatement notices or infringement notices in relation to the minor non-compliant effects however, abatement notices may have been issued to mitigate an identified potential for an environmental effect to occur.

For example:

- High suspended solid values recorded in discharge samples however, the discharge was to land or to receiving waters that were in high flow at the time;
- Strong odour beyond boundary but no residential properties or other recipient nearby.

Improvement required: Likely or actual adverse effects of activities on the receiving environment were more than minor, but not substantial. There were some issues noted during monitoring, from self-reports, or during investigations of incidents reported to the Council by a third party. Cumulative adverse effects of a persistent minor non-compliant activity could elevate a minor issue to this level. Abatement notices and infringement notices may have been issued in respect of effects.

Poor: Likely or actual adverse effects of activities on the receiving environment were significant. There were some items noted during monitoring, from self-reports, or during investigations of incidents reported to the Council by a third party. Cumulative adverse effects of a persistent moderate non-compliant activity could elevate an 'improvement required' issue to this level. Typically there were grounds for either a prosecution or an infringement notice in respect of effects.

Administrative performance

High: The administrative requirements of the resource consents were met, or any failure to do this had trivial consequences and were addressed promptly and co-operatively.

Good: Perhaps some administrative requirements of the resource consents were not met at a particular time however, this was addressed without repeated interventions from the Council staff. Alternatively adequate reason was provided for matters such as the no or late provision of information, interpretation of 'best practical option' for avoiding potential effects, etc.

Improvement required: Repeated interventions to meet the administrative requirements of the resource consents were made by Council staff. These matters took some time to resolve, or remained unresolved at the end of the period under review. The Council may have issued an abatement notice to attain compliance.

Poor: Material failings to meet the administrative requirements of the resource consents. Significant intervention by the Council was required. Typically there were grounds for an infringement notice.

Appendix III

Certificates of analysis
(groundwater)



Certificate of Analysis

Client: Taranaki Regional Council	Lab No: 2539666	SPV1
Contact: Jane Harvey	Date Received: 26-Feb-2021	
C/- Taranaki Regional Council	Date Reported: 05-Mar-2021	
Private Bag 713	Quote No: 47915	
Stratford 4352	Order No: 72831	
	Client Reference: #6601 - Greymouth Turangi-B 1yr PF/3 mnth PF/Pre-Frac	
	Submitted By: Kelby Clements	

Sample Type: Aqueous

Sample Name:	TRC210881 (GND3061) 25-Feb-2021 11:05 am				
Lab Number:	2539666.1				
Individual Tests					
Sum of Anions	meq/L	3.8	-	-	-
Sum of Cations	meq/L	3.7	-	-	-
pH	pH Units	7.4	-	-	-
Total Alkalinity	g/m ³ as CaCO ₃	167	-	-	-
Bicarbonate	g/m ³ at 25°C	200	-	-	-
Total Hardness	g/m ³ as CaCO ₃	108	-	-	-
Electrical Conductivity (EC)	mS/m	36.0	-	-	-
Total Dissolved Solids (TDS)	g/m ³	220	-	-	-
Sample Temperature*†	°C	17.1	-	-	-
Dissolved Barium	g/m ³	0.033	-	-	-
Dissolved Calcium	g/m ³	24	-	-	-
Dissolved Copper	g/m ³	< 0.0005	-	-	-
Dissolved Iron	g/m ³	4.5	-	-	-
Dissolved Magnesium	g/m ³	12.0	-	-	-
Dissolved Manganese	g/m ³	0.23	-	-	-
Dissolved Mercury	g/m ³	< 0.00008	-	-	-
Dissolved Nickel	g/m ³	< 0.0005	-	-	-
Dissolved Potassium	g/m ³	7.0	-	-	-
Dissolved Sodium	g/m ³	28	-	-	-
Dissolved Zinc	g/m ³	0.0052	-	-	-
Bromide	g/m ³	0.06	-	-	-
Chloride	g/m ³	16.3	-	-	-
Nitrite-N	g/m ³	0.004	-	-	-
Nitrate-N	g/m ³	0.012	-	-	-
Nitrate-N + Nitrite-N	g/m ³	0.016	-	-	-
Sulphate	g/m ³	< 0.5	-	-	-
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	< 4	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 4	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 4	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	TRC210881 (GND3061) 25-Feb-2021 11:05 am				
Lab Number:	2539666.1				
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	< 0.0010	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Formaldehyde in Water by DNPH & LCMSMS					
Formaldehyde	g/m ³	< 0.02	-	-	-
Gases in groundwater					
Ethane	g/m ³	< 0.003	-	-	-
Ethylene	g/m ³	< 0.004	-	-	-
Methane	g/m ³	8.3	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.10	-	-	-
C10 - C14	g/m ³	< 0.2	-	-	-
C15 - C36	g/m ³	< 0.4	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7	-	-	-

Analyst's Comments

† Customer supplied data. Please note: Hill Laboratories cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 28-Feb-2021 and 05-Mar-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	3343397	SPV1
Contact:	Jane Harvey C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	16-Aug-2023	
		Date Reported:	28-Aug-2023	
		Quote No:	47915	
		Order No:	4500011519	
		Client Reference:	Groundwater	
		Submitted By:	Sarah Avery	

Sample Type: Aqueous

Sample Name:	TRC2313713 (GND3061) 15-Aug-2023 10:38 am
Lab Number:	3343397.1

Individual Tests		
Sum of Anions	meq/L	3.6
Sum of Cations	meq/L	3.9
pH	pH Units	7.4
Total Alkalinity	g/m ³ as CaCO ₃	159
Bicarbonate	g/m ³ at 25°C	194
Total Hardness	g/m ³ as CaCO ₃	127
Electrical Conductivity (EC)	mS/m	34.1
Total Dissolved Solids (TDS)	g/m ³	240
Sample Temperature*†	°C	14.9
Dissolved Barium	g/m ³	0.056
Dissolved Calcium	g/m ³	30
Dissolved Copper	g/m ³	< 0.0005
Dissolved Iron	g/m ³	9.6
Dissolved Magnesium	g/m ³	12.7
Dissolved Manganese	g/m ³	0.40
Dissolved Mercury	g/m ³	< 0.00008
Dissolved Nickel	g/m ³	< 0.0005
Dissolved Potassium	g/m ³	5.1
Dissolved Sodium	g/m ³	21
Dissolved Zinc	g/m ³	0.0022
Bromide	g/m ³	0.08
Chloride	g/m ³	15.5
Nitrite-N	g/m ³	0.005
Nitrate-N	g/m ³	0.014
Nitrate-N + Nitrite-N	g/m ³	0.019
Sulphate	g/m ³	< 0.5
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 4
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 4
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 2
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	< 0.0010
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	< 0.002
o-Xylene	g/m ³	< 0.0010

Sample Type: Aqueous		
Sample Name:	TRC2313713 (GND3061) 15-Aug-2023 10:38 am	
Lab Number:	3343397.1	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.02
Gases in groundwater		
Ethane	g/m ³	< 0.003
Ethylene	g/m ³	< 0.004
Methane	g/m ³	14.5
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.10
C10 - C14	g/m ³	< 0.2
C15 - C36	g/m ³	< 0.4
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7

Analyst's Comments

† Customer supplied data. Please note: Hill Labs cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-Aug-2023 and 28-Aug-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Martin Cowell - BSc
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	3550124	SPV1
Contact:	Elizabeth Fynan C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	19-Apr-2024	
		Date Reported:	20-May-2024	
		Quote No:	47915	
		Order No:	300852	
		Client Reference:	#9429 - Turangi-B 1 Yr PF GW April 2024	
		Submitted By:	Paloma Craig	

Sample Type: Aqueous

Sample Name:	TRC2418074 (GND3061) 18-Apr-2024 11:45 am
Lab Number:	3550124.1

Individual Tests		
Gases in Ground Water**		See attached report
Sum of Anions	meq/L	3.9
Sum of Cations	meq/L	4.1
pH	pH Units	7.0
Total Alkalinity	g/m ³ as CaCO ₃	171
Bicarbonate	g/m ³ at 25°C	210
Total Hardness	g/m ³ as CaCO ₃	127
Electrical Conductivity (EC)	mS/m	36.2
Total Dissolved Solids (TDS)	g/m ³	270
Sample Temperature*†	°C	16.0
Dissolved Barium	g/m ³	0.048
Dissolved Calcium	g/m ³	29
Dissolved Copper	g/m ³	< 0.0005
Dissolved Iron	g/m ³	8.1
Dissolved Magnesium	g/m ³	13.4
Dissolved Manganese	g/m ³	0.31
Dissolved Mercury	g/m ³	< 0.00008
Dissolved Nickel	g/m ³	< 0.0005
Dissolved Potassium	g/m ³	6.2
Dissolved Sodium	g/m ³	26
Dissolved Zinc	g/m ³	0.0093
Bromide	g/m ³	0.07
Chloride	g/m ³	16.7
Nitrite-N	g/m ³	0.005 #1
Nitrate-N	g/m ³	< 0.002
Nitrate-N + Nitrite-N	g/m ³	0.003 #1
Sulphate	g/m ³	< 0.5
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 4
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 4
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 2

Sample Type: Aqueous		
Sample Name:	TRC2418074 (GND3061) 18-Apr-2024 11:45 am	
Lab Number:	3550124.1	
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	< 0.0010
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	< 0.002
o-Xylene	g/m ³	< 0.0010
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	0.02
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.10
C10 - C14	g/m ³	< 0.2
C15 - C36	g/m ³	< 0.4
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7

Analyst's Comments

† Customer supplied data. Please note: Hill Labs cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

‡ Analysis subcontracted to an external provider. Refer to the Summary of Methods section for more details.

#1 It has been noted that the result for Nitrite-N was greater than that for Nitrate-N + Nitrite-N, but within the analytical variation of these methods.

Appendix No.1 - Analytica Report

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Gases in Ground Water*	See attached report. Subcontracted to ALS Environmental - Brisbane.	-	1
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E : Online Edition.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E : Online Edition.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B (modified) : Online Edition. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) : Online Edition.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D : Online Edition.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B : Online Edition.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B : Online Edition.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) : Online Edition.	10 g/m ³	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) : Online Edition.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - Nitrite-N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) : Online Edition.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID analysis.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID analysis.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 20-Apr-2024 and 20-May-2024. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Ara Heron BSc (Tech)
Client Services Manager - Environmental



CERTIFICATE OF ANALYSIS

Work Order	: EB2415788	Page	: 1 of 2
Client	: ANALYTICA LABORATORIES LIMITED	Laboratory	: Environmental Division Brisbane
Contact	: Default reports	Contact	: Customer Services EB
Address	: RUAKURA RESEARCH CENTRE 10 Bisley Road HAMILTON WAIKATO, NZ 3240	Address	: 2 Byth Street Stafford QLD Australia 4053
Telephone	: ----	Telephone	: +61-7-3243 7222
Project	: 24-14611	Date Samples Received	: 10-May-2024 12:00
Order number	: ----	Date Analysis Commenced	: 15-May-2024
C-O-C number	: ----	Issue Date	: 17-May-2024 17:18
Sampler	: ----		
Site	: ----		
Quote number	: EN/222		
No. of samples received	: 1		
No. of samples analysed	: 1		



This report supersedes any previous report(s) with this reference. Results apply to the sample(s) as submitted, unless the sampling was conducted by ALS. This document shall not be reproduced, except in full.

This Certificate of Analysis contains the following information:

- General Comments
- Analytical Results

Additional information pertinent to this report will be found in the following separate attachments: Quality Control Report, QA/QC Compliance Assessment to assist with Quality Review and Sample Receipt Notification.

Signatories

This document has been electronically signed by the authorized signatories below. Electronic signing is carried out in compliance with procedures specified in 21 CFR Part 11.

<i>Signatories</i>	<i>Position</i>	<i>Accreditation Category</i>
Alex Rossi	Organic Chemist	Sydney Organics, Smithfield, NSW



Page : 2 of 2
 Work Order : EB2415788
 Client : ANALYTICA LABORATORIES LIMITED
 Project : 24-14611

General Comments

The analytical procedures used by ALS have been developed from established internationally recognised procedures such as those published by the USEPA, APHA, AS and NEPM. In house developed procedures are fully validated and are often at the client request.

Where moisture determination has been performed, results are reported on a dry weight basis.

Where a reported less than (<) result is higher than the LOR, this may be due to primary sample extract/digestate dilution and/or insufficient sample for analysis.

Where the LOR of a reported result differs from standard LOR, this may be due to high moisture content, insufficient sample (reduced weight employed) or matrix interference.

When sampling time information is not provided by the client, sampling dates are shown without a time component. In these instances, the time component has been assumed by the laboratory for processing purposes.

Where a result is required to meet compliance limits the associated uncertainty must be considered. Refer to the ALS Contract for details.

Key : CAS Number = CAS registry number from database maintained by Chemical Abstracts Services. The Chemical Abstracts Service is a division of the American Chemical Society.
 LOR = Limit of reporting
 ^ = This result is computed from individual analyte detections at or above the level of reporting
 ø = ALS is not NATA accredited for these tests.
 ~ = Indicates an estimated value.

- Analysis is conducted by ALS Environmental, Sydney, NATA accreditation no. 825, Site No. 10911 (Micro site no. 14913).

Analytical Results

Sub-Matrix: WATER
 (Matrix: WATER)

Sample ID

24-14611-1 3550124.1

Sampling date / time

10-May-2024 00:00

Compound

CAS Number

LOR

Unit

EB2415788-001

Result

EP033: C1 - C4 Hydrocarbon Gases

Compound	CAS Number	LOR	Unit	Result	----	----	----	----
Methane	74-82-8	1	µg/L	8760	----	----	----	----
Ethene	74-85-1	1	µg/L	<1	----	----	----	----
Ethane	74-84-0	1	µg/L	<1	----	----	----	----
Propene	115-07-1	1	µg/L	<1	----	----	----	----
Propane	74-98-6	1	µg/L	<1	----	----	----	----
Butene	25167-67-3	1	µg/L	<1	----	----	----	----
Butane	106-97-8	1	µg/L	<1	----	----	----	----

Inter-Laboratory Testing

Analysis conducted by ALS Sydney, NATA accreditation no. 825, site no. 10911 (Chemistry) 14913 (Biology).

(WATER) EP033: C1 - C4 Hydrocarbon Gases



Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	3242369	SPV1
Contact:	Sarah Avery C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	15-Apr-2023	
		Date Reported:	24-Apr-2023	
		Quote No:	47915	
		Order No:	4500007241	
		Client Reference:	#8465 - Turangi-B HF 3 month PF GW April 2023	
		Submitted By:	Peter Hayes	

Sample Type: Aqueous

Sample Name:	TRC2311843 (GND3061) 14-Apr-2023 12:30 pm		
Lab Number:	3242369.1		
Individual Tests			
Sum of Anions	meq/L		3.8
Sum of Cations	meq/L		4.0
pH	pH Units		7.4
Total Alkalinity	g/m ³ as CaCO ₃		165
Bicarbonate	g/m ³ at 25°C		200
Total Hardness	g/m ³ as CaCO ₃		120
Electrical Conductivity (EC)	mS/m		35.3
Total Dissolved Solids (TDS)	g/m ³		240
Sample Temperature*†	°C		16.0
Dissolved Barium	g/m ³		0.048
Dissolved Calcium	g/m ³		27
Dissolved Copper	g/m ³		< 0.0005
Dissolved Iron	g/m ³		8.1
Dissolved Magnesium	g/m ³		12.5
Dissolved Manganese	g/m ³		0.31
Dissolved Mercury	g/m ³		< 0.00008
Dissolved Nickel	g/m ³		< 0.0005
Dissolved Potassium	g/m ³		6.0
Dissolved Sodium	g/m ³		27
Dissolved Zinc	g/m ³		< 0.0010
Bromide	g/m ³		0.10
Chloride	g/m ³		17.1
Nitrite-N	g/m ³		0.006
Nitrate-N	g/m ³		0.006
Nitrate-N + Nitrite-N	g/m ³		0.011
Sulphate	g/m ³		< 0.5
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 4
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 4
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 2
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		< 0.0010
Toluene	g/m ³		< 0.0010
Ethylbenzene	g/m ³		< 0.0010
m&p-Xylene	g/m ³		< 0.002
o-Xylene	g/m ³		< 0.0010



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous		
Sample Name:	TRC2311843 (GND3061) 14-Apr-2023 12:30 pm	
Lab Number:	3242369.1	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.02
Gases in groundwater		
Ethane	g/m ³	< 0.003
Ethylene	g/m ³	< 0.004
Methane	g/m ³	12.3
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.10
C10 - C14	g/m ³	< 0.2
C15 - C36	g/m ³	< 0.4
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7

Analyst's Comments

† Customer supplied data. Please note: Hill Laboratories cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 18-Apr-2023 and 24-Apr-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Kim Harrison MSc
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	3373767	SPV1
Contact:	Jane Harvey C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	28-Sep-2023	
		Date Reported:	05-Oct-2023	
		Quote No:	47915	
		Order No:	4500011519	
		Client Reference:	#8876 - Turangi-B 1yr PF GW Sept 2023	
		Submitted By:	Sarah Avery	

Sample Type: Aqueous

Sample Name:	TRC2314267 GND3061 27-Sep-2023 10:20 am
Lab Number:	3373767.1

Individual Tests		
Sum of Anions	meq/L	3.7
Sum of Cations	meq/L	4.2
pH	pH Units	7.0
Total Alkalinity	g/m ³ as CaCO ₃	159
Bicarbonate	g/m ³ at 25°C	194
Total Hardness	g/m ³ as CaCO ₃	133
Electrical Conductivity (EC)	mS/m	35.6
Total Dissolved Solids (TDS)	g/m ³	250
Sample Temperature*†	°C	14.8
Dissolved Barium	g/m ³	0.065
Dissolved Calcium	g/m ³	31
Dissolved Copper	g/m ³	< 0.0005
Dissolved Iron	g/m ³	12.1
Dissolved Magnesium	g/m ³	13.8
Dissolved Manganese	g/m ³	0.44
Dissolved Mercury	g/m ³	< 0.00008
Dissolved Nickel	g/m ³	< 0.0005
Dissolved Potassium	g/m ³	5.1
Dissolved Sodium	g/m ³	22
Dissolved Zinc	g/m ³	0.0035
Bromide	g/m ³	0.08
Chloride	g/m ³	16.6
Nitrite-N	g/m ³	0.005
Nitrate-N	g/m ³	< 0.002
Nitrate-N + Nitrite-N	g/m ³	0.005
Sulphate	g/m ³	< 0.5
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 4
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 4
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 2
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	< 0.0010
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	< 0.002
o-Xylene	g/m ³	< 0.0010

Sample Type: Aqueous		
Sample Name:	TRC2314267 GND3061 27-Sep-2023 10:20 am	
Lab Number:	3373767.1	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.02
Gases in groundwater		
Ethane	g/m ³	< 0.003
Ethylene	g/m ³	< 0.004
Methane	g/m ³	15.7
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.10
C10 - C14	g/m ³	< 0.2
C15 - C36	g/m ³	< 0.4
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7

Analyst's Comments

† Customer supplied data. Please note: Hill Labs cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E : Online Edition.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E : Online Edition.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B (modified) : Online Edition. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) : Online Edition.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D : Online Edition.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B : Online Edition.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B : Online Edition.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) : Online Edition.	10 g/m ³	1
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B : Online Edition.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) : Online Edition.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - Nitrite-N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) : Online Edition.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) : Online Edition.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 28-Sep-2023 and 05-Oct-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis

Client:	Taranaki Regional Council	Lab No:	2654099	SPV1
Contact:	Jane Harvey C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	10-Jul-2021	
		Date Reported:	20-Jul-2021	
		Quote No:	47915	
		Order No:	4500002828	
		Client Reference:	#6847- Turangi-B interim frac	
		Submitted By:	Angela Collins	

Sample Type: Aqueous

Sample Name:	TRC212297 (GND3061) 09-Jul-2021 11:20 am				
Lab Number:	2654099.1				

Individual Tests

Sum of Anions	meq/L	3.7	-	-	-	-
Sum of Cations	meq/L	3.9	-	-	-	-
pH	pH Units	6.9	-	-	-	-
Total Alkalinity	g/m ³ as CaCO ₃	159	-	-	-	-
Bicarbonate	g/m ³ at 25°C	194	-	-	-	-
Total Hardness	g/m ³ as CaCO ₃	125	-	-	-	-
Electrical Conductivity (EC)	mS/m	36.1	-	-	-	-
Total Dissolved Solids (TDS)	g/m ³	240	-	-	-	-
Sample Temperature*†	°C	15.0	-	-	-	-
Dissolved Barium	g/m ³	0.064	-	-	-	-
Dissolved Calcium	g/m ³	30	-	-	-	-
Dissolved Copper	g/m ³	< 0.0005	-	-	-	-
Dissolved Iron	g/m ³	10.8	-	-	-	-
Dissolved Magnesium	g/m ³	12.3	-	-	-	-
Dissolved Manganese	g/m ³	0.48	-	-	-	-
Dissolved Mercury	g/m ³	< 0.00008	-	-	-	-
Dissolved Nickel	g/m ³	0.0005	-	-	-	-
Dissolved Potassium	g/m ³	5.2	-	-	-	-
Dissolved Sodium	g/m ³	21	-	-	-	-
Dissolved Zinc	g/m ³	0.0044	-	-	-	-
Bromide	g/m ³	0.09	-	-	-	-
Chloride	g/m ³	16.4	-	-	-	-
Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Nitrate-N	g/m ³	< 0.02	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Sulphate	g/m ³	1.0	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 4	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 4	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 2	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	TRC212297 (GND3061) 09-Jul-2021 11:20 am				
Lab Number:	2654099.1				
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	< 0.0010	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Formaldehyde in Water by DNPH & LCMSMS					
Formaldehyde	g/m ³	0.02	-	-	-
Gases in groundwater					
Ethane	g/m ³	< 0.003	-	-	-
Ethylene	g/m ³	< 0.004	-	-	-
Methane	g/m ³	14.2	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.10	-	-	-
C10 - C14	g/m ³	< 0.2	-	-	-
C15 - C36	g/m ³	< 0.4	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7	-	-	-

Analyst's Comments

It has been noted that the spike for Methanol on sample 2654099.1, was run as part of our in-house QC procedure, had a lower than expected recovery at 44%. Therefore the result may be underestimated.

† Customer supplied data. Please note: Hill Laboratories cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 12-Jul-2021 and 20-Jul-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	2812323	SPV1
Contact:	Jane Harvey C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	24-Dec-2021	
		Date Reported:	07-Jan-2022	
		Quote No:	47915	
		Order No:	4500002828	
		Client Reference:	#7296- GPL Turangi-B 3 month PF+ Pre-frac Dec 2021	
		Submitted By:	Sarah Larkin	

Interim Report

This is an interim report, prepared before all test results are completed. As all final Q.C. checks may not have been possible, it is not regarded as an official certificate of analysis. The final, official report will be issued upon completion of all tests.

Sample Type: Aqueous

Sample Name:	TRC214610 (GND3061) 23-Dec-2021 9:45 am				
Lab Number:	2812323.1				

Individual Tests

Sum of Anions	meq/L	3.5	-	-	-	-
Sum of Cations	meq/L	3.6	-	-	-	-
pH	pH Units	7.1	-	-	-	-
Total Alkalinity	g/m ³ as CaCO ₃	149	-	-	-	-
Bicarbonate	g/m ³ at 25°C	182	-	-	-	-
Total Hardness	g/m ³ as CaCO ₃	112	-	-	-	-
Electrical Conductivity (EC)	mS/m	32.7	-	-	-	-
Total Dissolved Solids (TDS)	g/m ³	240	-	-	-	-
Sample Temperature†	°C	17.0	-	-	-	-
Dissolved Barium	g/m ³	0.047	-	-	-	-
Dissolved Calcium	g/m ³	26	-	-	-	-
Dissolved Copper	g/m ³	< 0.0005	-	-	-	-
Dissolved Iron	g/m ³	8.3	-	-	-	-
Dissolved Magnesium	g/m ³	11.4	-	-	-	-
Dissolved Manganese	g/m ³	0.37	-	-	-	-
Dissolved Mercury	g/m ³	< 0.00008	-	-	-	-
Dissolved Nickel	g/m ³	< 0.0005	-	-	-	-
Dissolved Potassium	g/m ³	5.5	-	-	-	-
Dissolved Sodium	g/m ³	21	-	-	-	-
Dissolved Zinc	g/m ³	0.0113	-	-	-	-
Bromide	g/m ³	0.09	-	-	-	-
Chloride	g/m ³	17.1	-	-	-	-
Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Nitrate-N	g/m ³	< 0.02	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Sulphate	g/m ³	< 0.5	-	-	-	-
Ethylene Glycol in Water						
Ethylene glycol	g/m ³	< 4	-	-	-	-
Propylene Glycol in Water						
Propylene glycol	g/m ³	< 4	-	-	-	-
Methanol in Water - Aqueous Solvents						
Methanol	g/m ³	In Progress	-	-	-	-
BTEX in Water by Headspace GC-MS						
Benzene	g/m ³	< 0.0010	-	-	-	-
Toluene	g/m ³	< 0.0010	-	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-	-

Sample Type: Aqueous

Sample Name:	TRC214610 (GND3061) 23-Dec-2021 9:45 am				
Lab Number:	2812323.1				
BTEX in Water by Headspace GC-MS					
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Formaldehyde in Water by DNPH & LCMSMS					
Formaldehyde	g/m ³	< 0.02	-	-	-
Gases in groundwater					
Ethane	g/m ³	< 0.003	-	-	-
Ethylene	g/m ³	< 0.004	-	-	-
Methane	g/m ³	11.2	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.10	-	-	-
C10 - C14	g/m ³	< 0.2	-	-	-
C15 - C36	g/m ³	< 0.4	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7	-	-	-

Analyst's Comments

† Customer supplied data. Please note: Hill Laboratories cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

#1 Severe matrix interferences required that a dilution be performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NOxN /NO2N analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N. Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1
Sample Temperature	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 24-Dec-2021 and 06-Jan-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Carole Rodgers-Carroll BA, NZCS
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 3

Client:	Taranaki Regional Council	Lab No:	3013927	SPV1
Contact:	Jane Harvey C/- Taranaki Regional Council Private Bag 713 Stratford 4352	Date Received:	15-Jun-2022	
		Date Reported:	22-Jun-2022	
		Quote No:	47915	
		Order No:	4500002828	
		Client Reference:	#7622 - GPL Turangi-B 3 month PF + 1 Yr PF GW June 2022	
		Submitted By:	Adele Bittner	

Sample Type: Aqueous

Sample Name:	TRC226761 (GND3061) 14-Jun-2022 12:47 pm				
Lab Number:	3013927.1				

Individual Tests

Sum of Anions	meq/L	3.3	-	-	-	-
Sum of Cations	meq/L	3.4	-	-	-	-
pH	pH Units	7.1	-	-	-	-
Total Alkalinity	g/m ³ as CaCO ₃	141	-	-	-	-
Bicarbonate	g/m ³ at 25°C	172	-	-	-	-
Total Hardness	g/m ³ as CaCO ₃	105	-	-	-	-
Electrical Conductivity (EC)	mS/m	31.2	-	-	-	-
Total Dissolved Solids (TDS)	g/m ³	260	-	-	-	-
Sample Temperature*†	°C	15.0	-	-	-	-
Dissolved Barium	g/m ³	0.051	-	-	-	-
Dissolved Calcium	g/m ³	24	-	-	-	-
Dissolved Copper	g/m ³	< 0.0005	-	-	-	-
Dissolved Iron	g/m ³	9.4	-	-	-	-
Dissolved Magnesium	g/m ³	10.8	-	-	-	-
Dissolved Manganese	g/m ³	0.38	-	-	-	-
Dissolved Mercury	g/m ³	< 0.00008	-	-	-	-
Dissolved Nickel	g/m ³	0.0006	-	-	-	-
Dissolved Potassium	g/m ³	4.2	-	-	-	-
Dissolved Sodium	g/m ³	18.8	-	-	-	-
Dissolved Zinc	g/m ³	0.0116	-	-	-	-
Bromide	g/m ³	0.07	-	-	-	-
Chloride	g/m ³	16.6	-	-	-	-
Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Nitrate-N	g/m ³	< 0.02	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.02 #1	-	-	-	-
Sulphate	g/m ³	< 0.5	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 4	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 4	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 2	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	TRC226761 (GND3061) 14-Jun-2022 12:47 pm				
Lab Number:	3013927.1				

BTEX in Water by Headspace GC-MS						
Benzene	g/m ³	< 0.0010	-	-	-	-
Toluene	g/m ³	0.0014	-	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-	-
Formaldehyde in Water by DNPH & LCMSMS						
Formaldehyde	g/m ³	< 0.02	-	-	-	-
Gases in groundwater						
Ethane	g/m ³	< 0.003	-	-	-	-
Ethylene	g/m ³	< 0.004	-	-	-	-
Methane	g/m ³	11.7	-	-	-	-
Total Petroleum Hydrocarbons in Water						
C7 - C9	g/m ³	< 0.10	-	-	-	-
C10 - C14	g/m ³	< 0.2	-	-	-	-
C15 - C36	g/m ³	< 0.4	-	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 0.7	-	-	-	-

Analyst's Comments

† Customer supplied data. Please note: Hill Laboratories cannot be held responsible for the validity of this customer supplied data, or any subsequent calculations that rely on this information.

#1 Severe matrix interferences required that a dilution be performed prior to analysis of this sample, resulting in a detection limit higher than that normally achieved for the NO2N, NO3N and NOxN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total anions for anion/cation balance check	Calculation: sum of anions as mEq/L calculated from Alkalinity (bicarbonate), Chloride and Sulphate. Nitrate-N, Nitrite-N, Fluoride, Dissolved Reactive Phosphorus and Cyanide also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.07 meq/L	1
Total cations for anion/cation balance check	Sum of cations as mEq/L calculated from Sodium, Potassium, Calcium and Magnesium. Iron, Manganese, Aluminium, Zinc, Copper, Lithium, Total Ammoniacal-N and pH (H ⁺) also included in calculation if available. APHA 1030 E 23 rd ed. 2017.	0.05 meq/L	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Bicarbonate	Calculation: from alkalinity and pH, valid where TDS is not >500 mg/L and alkalinity is almost entirely due to hydroxides, carbonates or bicarbonates. APHA 4500-CO ₂ D 23 rd ed. 2017.	1.0 g/m ³ at 25°C	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	10 g/m ³	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Sample Temperature*	Temperature of the sample at the time of sampling, supplied by customer.	0.1 °C	1
Dissolved Barium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.005 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Mercury	0.45µm filtration, bromine oxidation followed by atomic fluorescence. US EPA Method 245.7, Feb 2005.	0.00008 g/m ³	1
Dissolved Nickel	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0005 g/m ³	1
Dissolved Potassium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.05 g/m ³	1
Dissolved Sodium	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.02 g/m ³	1
Dissolved Zinc	Filtered sample, ICP-MS, trace level. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Bromide	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.05 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate-N + Nitrite-N	Total oxidised nitrogen. Automated cadmium reduction, flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.002 g/m ³	1
Sulphate	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Gases in groundwater	Headspace GC-FID analysis. In-house.	0.002 - 0.003 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-Jun-2022 and 22-Jun-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Carole Rodgers-Carroll BA, NZCS
Client Services Manager - Environmental

Appendix IV

Certificates of analysis
(hydraulic fracturing fluids)

Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3293909	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	02-Jun-2023	
		Date Reported:	12-Jun-2023	
		Quote No:	81870	
		Order No:	260815	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	


Sample Type: Aqueous		
Sample Name:	Composite of Turangi 19 Stim 4 Return HF Fluid Start, Turangi 19 Stim 4 Return HF Fluid Middle, Turangi 19 Stim 4 Return HF Fluid End	
Lab Number:	3293909.4	
Individual Tests		
pH	pH Units	7.5
Total Alkalinity	g/m ³ as CaCO ₃	2,100
Total Hardness	g/m ³ as CaCO ₃	116
Electrical Conductivity (EC)	mS/m	1,100
Salinity*		6.2
Total Suspended Solids	g/m ³	270
Total Dissolved Solids (TDS)	g/m ³	8,900
Dissolved Barium	g/m ³	20
Dissolved Bromine	g/m ³	7.8
Dissolved Calcium	g/m ³	36
Dissolved Copper	g/m ³	0.005
Dissolved Iron	g/m ³	3.5
Dissolved Magnesium	g/m ³	6
Dissolved Manganese	g/m ³	0.57
Total Nickel*	g/m ³	0.040
Total Potassium*	g/m ³	73
Total Sodium*	g/m ³	2,300
Total Sulphur	g/m ³	10
Total Zinc*	g/m ³	0.34
Chloride	g/m ³	2,300
Nitrite-N	g/m ³	< 0.10 #1
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #1
Sulphate*	g/m ³	30
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 20
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	15.8
Toluene	g/m ³	14.9
Ethylbenzene	g/m ³	1.02
m&p-Xylene	g/m ³	5.9
o-Xylene	g/m ³	2.1

Sample Type: Aqueous

Sample Name:	Composite of Turangi 19 Stim 4 Return HF Fluid Start, Turangi 19 Stim 4 Return HF Fluid Middle, Turangi 19 Stim 4 Return HF Fluid End		
Lab Number:	3293909.4		
Formaldehyde in Water by DNPH & LCMSMS			
Formaldehyde	g/m ³	< 0.15	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	94	
C10 - C14	g/m ³	240	
C15 - C36	g/m ³	350	
Total hydrocarbons (C7 - C36)	g/m ³	690	

3293909.4

Composite of Turangi 19 Stim 4 Return HF Fluid Start, Turangi 19 Stim 4 Return HF Fluid Middle, Turangi 19 Stim 4 Return HF Fluid End
Client Chromatogram for TPH by FID

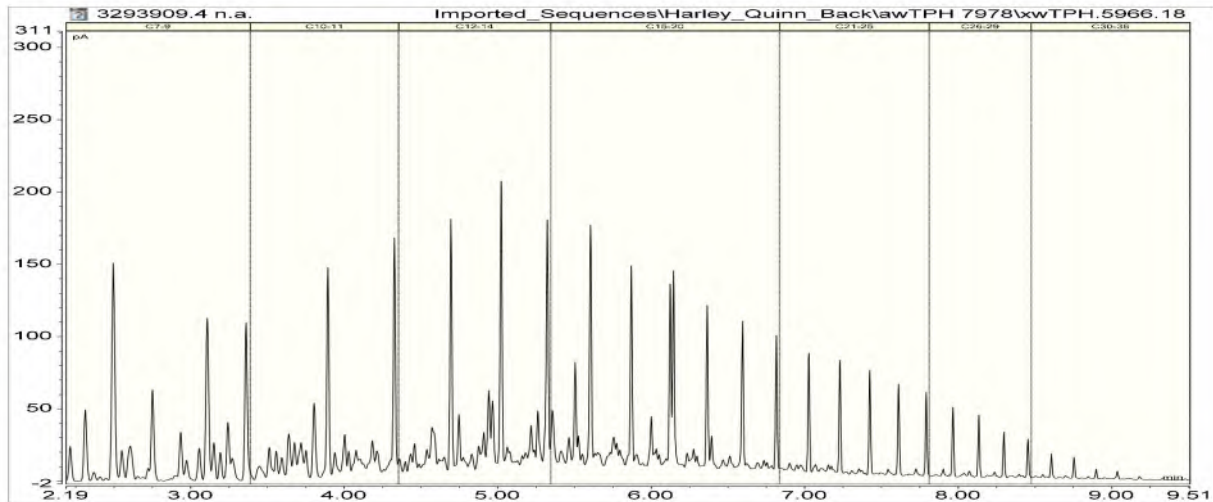**Analyst's Comments**

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 06-Jun-2023 and 12-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3293908	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	02-Jun-2023	
		Date Reported:	12-Jun-2023	
		Quote No:	81870	
		Order No:	260711	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous


Sample Name:	Composite of Turangi 19 Stim 3 Return HP Fluid Start, Turangi 19 Stim 3 Return HP Fluid Middle, Turangi 19 Stim 3 Return HP Fluid End
Lab Number:	3293908.4

Individual Tests		
pH	pH Units	7.0
Total Alkalinity	g/m ³ as CaCO ₃	870
Total Hardness	g/m ³ as CaCO ₃	280
Electrical Conductivity (EC)	mS/m	1,676
Salinity*		9.9
Total Suspended Solids	g/m ³	490
Total Dissolved Solids (TDS)	g/m ³	11,200
Dissolved Barium	g/m ³	22
Dissolved Bromine	g/m ³	19.7
Dissolved Calcium	g/m ³	82
Dissolved Copper	g/m ³	0.013
Dissolved Iron	g/m ³	9.4
Dissolved Magnesium	g/m ³	18
Dissolved Manganese	g/m ³	2.4
Total Nickel*	g/m ³	0.27
Total Potassium*	g/m ³	117
Total Sodium*	g/m ³	3,200
Total Sulphur	g/m ³	< 60
Total Zinc*	g/m ³	0.042
Chloride	g/m ³	4,900
Nitrite-N	g/m ³	< 0.10 #1
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #1
Sulphate*	g/m ³	< 160
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 20
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	40
Toluene	g/m ³	88
Ethylbenzene	g/m ³	11.7
m&p-Xylene	g/m ³	74
o-Xylene	g/m ³	23

Sample Type: Aqueous	
Sample Name:	Composite of Turangi 19 Stim 3 Return HP Fluid Start, Turangi 19 Stim 3 Return HP Fluid Middle, Turangi 19 Stim 3 Return HP Fluid End
Lab Number:	3293908.4
Formaldehyde in Water by DNPH & LCMSMS	
Formaldehyde	g/m ³ < 0.15
Total Petroleum Hydrocarbons in Water	
C7 - C9	g/m ³ 5,800
C10 - C14	g/m ³ 9,600
C15 - C36	g/m ³ 12,200
Total hydrocarbons (C7 - C36)	g/m ³ 28,000

3293908.4

Composite of Turangi 19 Stim 3 Return HP Fluid Start, Turangi 19 Stim 3 Return HP Fluid Middle, Turangi 19 Stim 3 Return HP Fluid End
Client Chromatogram for TPH by FID

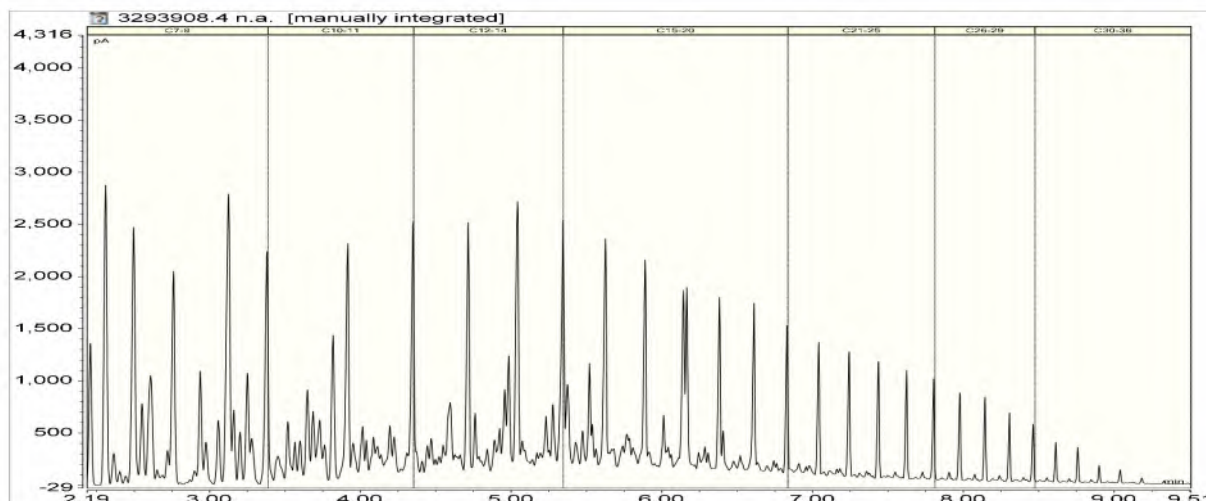

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 06-Jun-2023 and 12-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3283594	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	23-May-2023	
		Date Reported:	01-Jun-2023	
		Quote No:	81870	
		Order No:	260616	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous


Sample Name:	Composite of Turangi 19 Stim 2 Return HF Fluid Start, Turangi 19 Stim 2 Return HF Fluid Middle,, Turangi 19 Stim 2 Return HF Fluid End
Lab Number:	3283594.4

Individual Tests		
pH	pH Units	6.7
Total Alkalinity	g/m ³ as CaCO ₃	580
Total Hardness	g/m ³ as CaCO ₃	400
Electrical Conductivity (EC)	mS/m	1,756
Salinity*		10.3
Total Suspended Solids	g/m ³	590
Total Dissolved Solids (TDS)	g/m ³	12,400
Dissolved Barium	g/m ³	25
Dissolved Bromine	g/m ³	18.4
Dissolved Calcium	g/m ³	133
Dissolved Copper	g/m ³	0.049
Dissolved Iron	g/m ³	6.2
Dissolved Magnesium	g/m ³	16
Dissolved Manganese	g/m ³	2.1
Total Nickel*	g/m ³	0.53
Total Potassium*	g/m ³	139
Total Sodium*	g/m ³	3,600
Total Sulphur	g/m ³	< 60
Total Zinc*	g/m ³	0.144 #1
Chloride	g/m ³	6,000
Nitrite-N	g/m ³	< 0.10 #2
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #2
Sulphate*	g/m ³	< 160
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 20
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 110
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	35
Toluene	g/m ³	44
Ethylbenzene	g/m ³	3.8
m&p-Xylene	g/m ³	21
o-Xylene	g/m ³	5.9

Sample Type: Aqueous	
Sample Name:	Composite of Turangi 19 Stim 2 Return HF Fluid Start, Turangi 19 Stim 2 Return HF Fluid Middle,, Turangi 19 Stim 2 Return HF Fluid End
Lab Number:	3283594.4
Formaldehyde in Water by DNPH & LCMSMS	
Formaldehyde	g/m ³ < 0.15
Total Petroleum Hydrocarbons in Water	
C7 - C9	g/m ³ 1,090
C10 - C14	g/m ³ 1,490
C15 - C36	g/m ³ 1,760
Total hydrocarbons (C7 - C36)	g/m ³ 4,300

3283594.4

Composite of Turangi 19 Stim 2 Return HF Fluid Start, Turangi 19 Stim 2 Return HF Fluid Middle,, Turangi 19 Stim 2 Return HF Fluid End
Client Chromatogram for TPH by FID

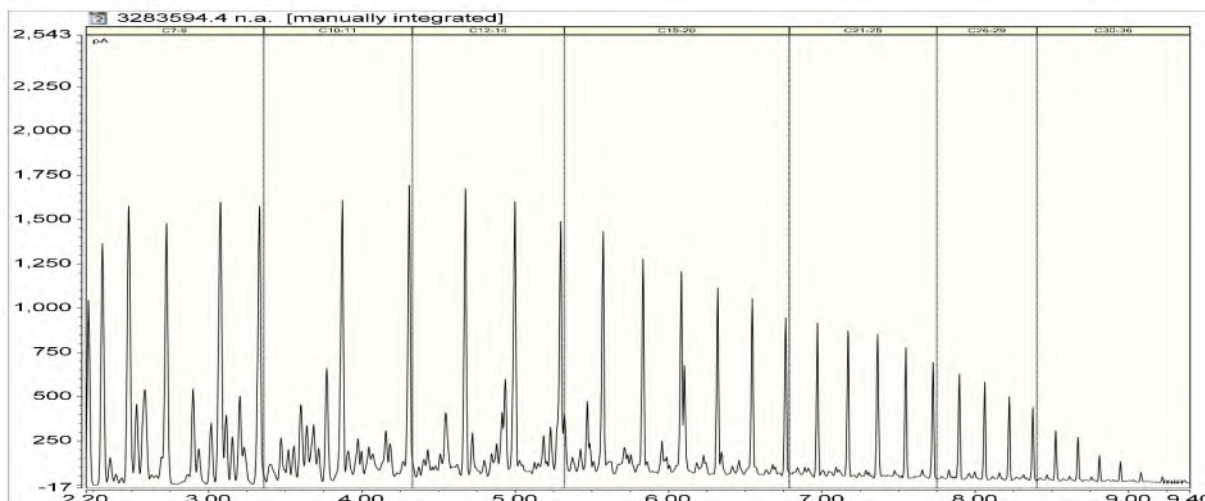

Analyst's Comments

#1 It should be noted that the replicate analyses performed on this sample as part of our in-house Quality Assurance procedures showed greater variation than would normally be expected. This may reflect the heterogeneity of the sample. The average of the results of the replicate analyses has been reported.

#2 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 24-May-2023 and 01-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes.

Ara Heron BSc (Tech)
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3283595	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	23-May-2023	
		Date Reported:	01-Jun-2023	
		Quote No:	81870	
		Order No:	260514	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 19 Stim 1 Return HF Fluid Start, Turangi 19 Stim 1 Return HF Fluid Middle, Turangi 19 Stim 1 Return HF Fluid End
Lab Number:	3283595.4


Individual Tests		
pH	pH Units	6.9
Total Alkalinity	g/m ³ as CaCO ₃	700
Total Hardness	g/m ³ as CaCO ₃	250
Electrical Conductivity (EC)	mS/m	1,512
Salinity*		8.8
Total Suspended Solids	g/m ³	560
Total Dissolved Solids (TDS)	g/m ³	9,500
Dissolved Barium	g/m ³	18.5
Dissolved Bromine	g/m ³	15.6
Dissolved Calcium	g/m ³	78
Dissolved Copper	g/m ³	0.56
Dissolved Iron	g/m ³	0.83
Dissolved Magnesium	g/m ³	14
Dissolved Manganese	g/m ³	1.84
Total Nickel*	g/m ³	1.17
Total Potassium*	g/m ³	158
Total Sodium*	g/m ³	3,100
Total Sulphur	g/m ³	< 60
Total Zinc*	g/m ³	1.83
Chloride	g/m ³	4,700
Nitrite-N	g/m ³	< 0.10 #1
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #1
Sulphate*	g/m ³	< 160
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 20
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 110
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	33
Toluene	g/m ³	45
Ethylbenzene	g/m ³	3.3
m&p-Xylene	g/m ³	18.2
o-Xylene	g/m ³	5.7

Sample Type: Aqueous

Sample Name:	Composite of Turangi 19 Stim 1 Return HF Fluid Start, Turangi 19 Stim 1 Return HF Fluid Middle, Turangi 19 Stim 1 Return HF Fluid End	
Lab Number:	3283595.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	2,200
C10 - C14	g/m ³	3,400
C15 - C36	g/m ³	5,000
Total hydrocarbons (C7 - C36)	g/m ³	10,600

3283595.4

Composite of Turangi 19 Stim 1 Return HF Fluid Start, Turangi 19 Stim 1 Return HF Fluid Middle, Turangi 19 Stim 1 Return HF Fluid End
Client Chromatogram for TPH by FID

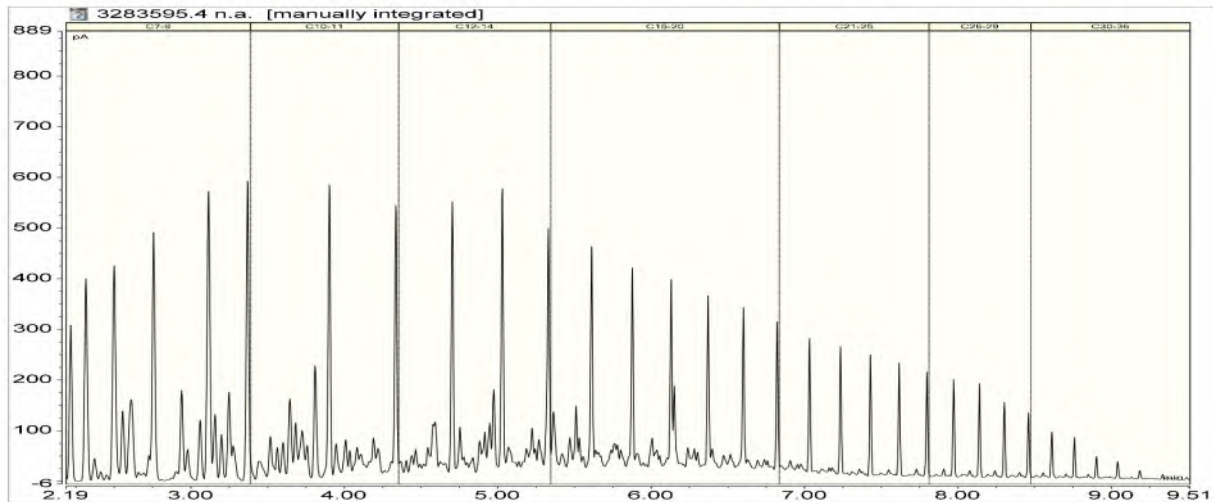

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 24-May-2023 and 01-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3300231	SPV1
Contact:	Fiona Campbell	Date Received:	13-Jun-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	20-Jun-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	261037	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 19 Stim 6 Prepumped HF Fluid 08-Jun-2023	
Lab Number:	3300231.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	820
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 400
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 110
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	0.0023
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	0.003
o-Xylene	g/m ³	0.0011
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	< 2
Total hydrocarbons (C7 - C36)	g/m ³	< 4

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 15-Jun-2023 and 20-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3297235	SPV1
Contact:	Fiona Campbell	Date Received:	08-Jun-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	13-Jun-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	260929	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous			
Sample Name:	Turangi 19 Stim 5 Prepumped HF Fluid 02-Jun-2023		
Lab Number:	3297235.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	860	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0031	
Toluene	g/m ³	0.0038	
Ethylbenzene	g/m ³	< 0.0010	
m&p-Xylene	g/m ³	0.003	
o-Xylene	g/m ³	0.0013	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 12-Jun-2023 and 13-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental


Certificate of Analysis

Page 1 of 2

Client: Greymouth Petroleum Limited	Lab No: 3290943	SPV1
Contact: Fiona Campbell	Date Received: 31-May-2023	
C/- Greymouth Petroleum Limited	Date Reported: 12-Jun-2023	
14 Connett Road West	Quote No: 85159	
Bell Block	Order No: 260815	
New Plymouth 4312	Client Reference: Hydraulic fracturing fluid testing	
	Submitted By: Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 19 Stim 4 Prepumped HF Fluid 26-May-2023	
Lab Number:	3290943.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	800
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	0.0013
Toluene	g/m ³	0.0038
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	0.003
o-Xylene	g/m ³	0.0014
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	3
Total hydrocarbons (C7 - C36)	g/m ³	< 4

3290943.1
 Turangi 19 Stim 4 Prepumped HF Fluid 26-May-2023
 Client Chromatogram for TPH by FID

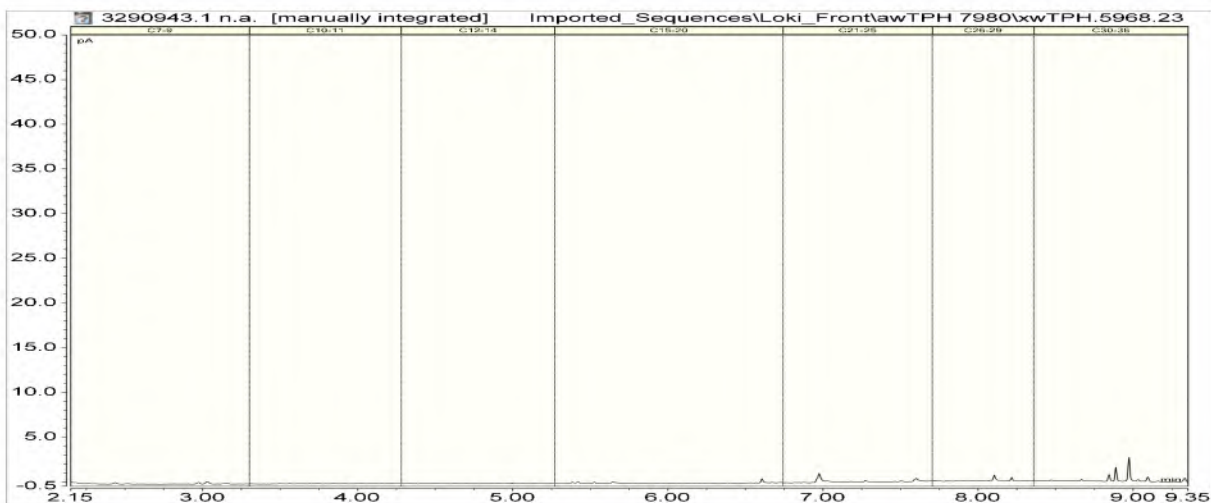

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 02-Jun-2023 and 12-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3279693	SPV1
Contact:	Fiona Campbell	Date Received:	18-May-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	31-May-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	260711	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 19 stim 3 prepumped HF Fluid 15-May-2023		
Lab Number:	3279693.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	650	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	< 0.0010	
Toluene	g/m ³	0.0021	
Ethylbenzene	g/m ³	< 0.0010	
m&p-Xylene	g/m ³	0.002	
o-Xylene	g/m ³	0.0011	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 24-May-2023 and 31-May-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Graham Corban MSc Tech (Hons)
Client Services Manager - Environmental




Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3273800	SPV1
Contact:	Fiona Campbell	Date Received:	12-May-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	19-May-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	260616	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 19 stim 2 prepumped HF fluid 08-May-2023	
Lab Number:	3273800.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	740
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 4
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 2
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	0.0030
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	0.003
o-Xylene	g/m ³	0.0012
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	3
Total hydrocarbons (C7 - C36)	g/m ³	< 4

3273800.1
Turangi 19 stim 2 prepumped HF fluid 08-May-2023
Client Chromatogram for TPH by FID

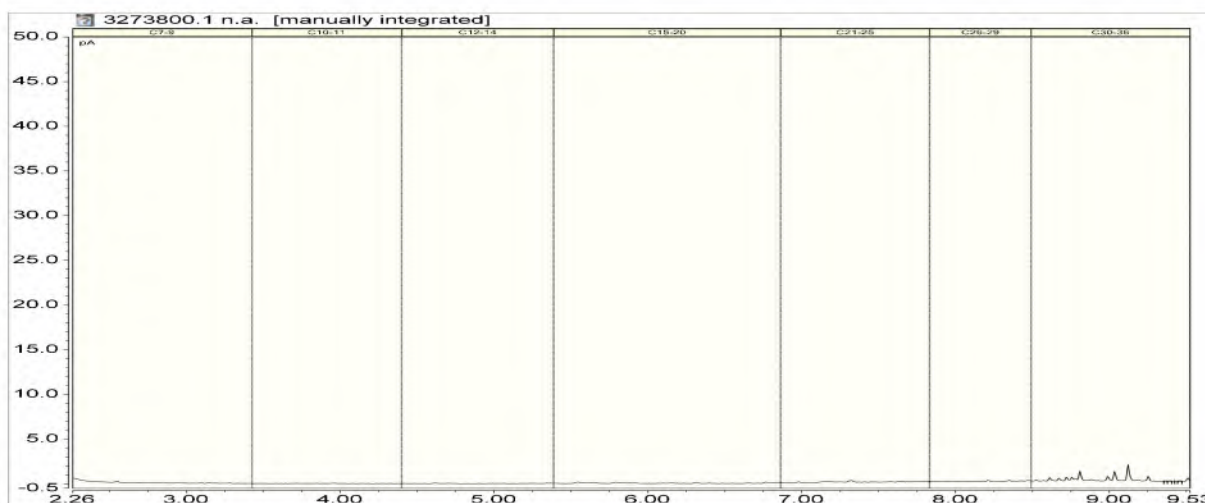

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-May-2023 and 19-May-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental




Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3267127	SPV1
Contact:	Fiona Campbell	Date Received:	05-May-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	19-May-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	260514	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 19 stim 1 prepumped HF Fluid 03-May-2023	
Lab Number:	3267127.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	77
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 4
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	< 0.0010
Toluene	g/m ³	0.0029
Ethylbenzene	g/m ³	< 0.0010
m&p-Xylene	g/m ³	0.003
o-Xylene	g/m ³	0.0011
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	2
Total hydrocarbons (C7 - C36)	g/m ³	< 4

3267127.1
Turangi 19 stim 1 prepumped HF Fluid 03-May-2023
Client Chromatogram for TPH by FID

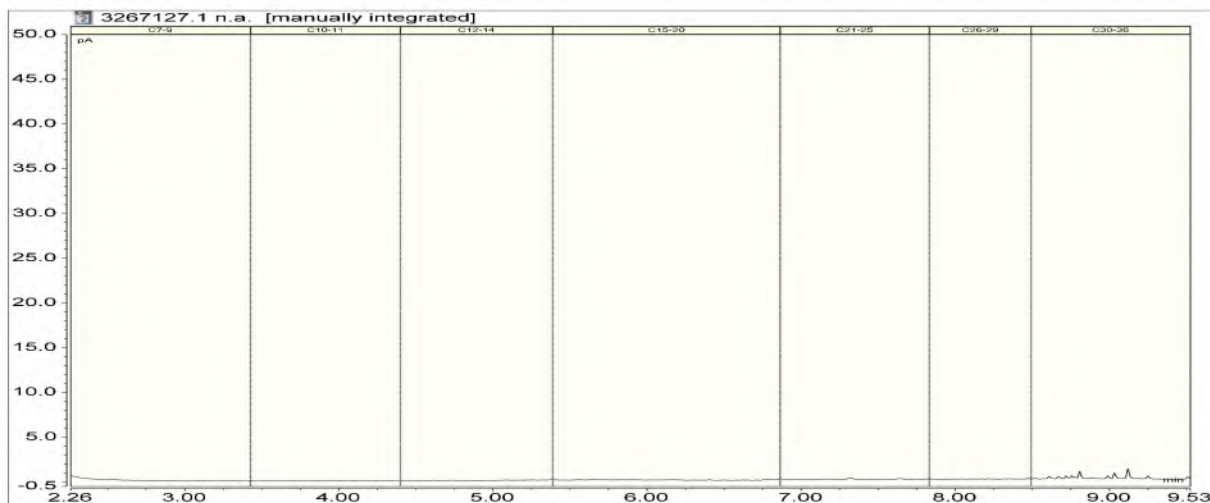

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 10-May-2023 and 19-May-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3179524	SPV1
Contact:	Fiona Campbell	Date Received:	22-Feb-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	06-Mar-2023	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	258471	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous


Sample Name:	Turangi 18 Stim 6 Return HF Fluid - Start 01-Feb-2023		
Lab Number:	3179524.1		
Individual Tests			
pH	pH Units		4.7
Total Alkalinity	g/m ³ as CaCO ₃		47 #1
Total Hardness	g/m ³ as CaCO ₃		82
Electrical Conductivity (EC)	mS/m		99.2
Salinity*			0.3
Total Suspended Solids	g/m ³		550
Total Dissolved Solids (TDS)	g/m ³		3,700
Dissolved Barium	g/m ³		0.078
Dissolved Bromine	g/m ³		< 0.5
Dissolved Calcium	g/m ³		21
Dissolved Copper	g/m ³		0.010
Dissolved Iron	g/m ³		1.42
Dissolved Magnesium	g/m ³		7
Dissolved Manganese	g/m ³		0.061
Total Nickel*	g/m ³		0.104
Total Potassium*	g/m ³		12.7
Total Sodium*	g/m ³		63
Total Sulphur	g/m ³		14
Total Zinc*	g/m ³		0.118
Chloride	g/m ³		210
Nitrite-N	g/m ³		< 0.10
Nitrate-N	g/m ³		0.18
Nitrate	g/m ³		0.8
Nitrate-N + Nitrite-N	g/m ³		0.19
Sulphate*	g/m ³		43
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 110
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		23
Toluene	g/m ³		8.5
Ethylbenzene	g/m ³		0.20
m&p-Xylene	g/m ³		0.92
o-Xylene	g/m ³		0.39



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous		
Sample Name:	Turangi 18 Stim 6 Return HF Fluid - Start 01-Feb-2023	
Lab Number:	3179524.1	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	17.0
C10 - C14	g/m ³	21
C15 - C36	g/m ³	21
Total hydrocarbons (C7 - C36)	g/m ³	60

3179524.1
 Turangi 18 Stim 6 Return HF Fluid - Start 01-Feb-2023
 Client Chromatogram for TPH by FID

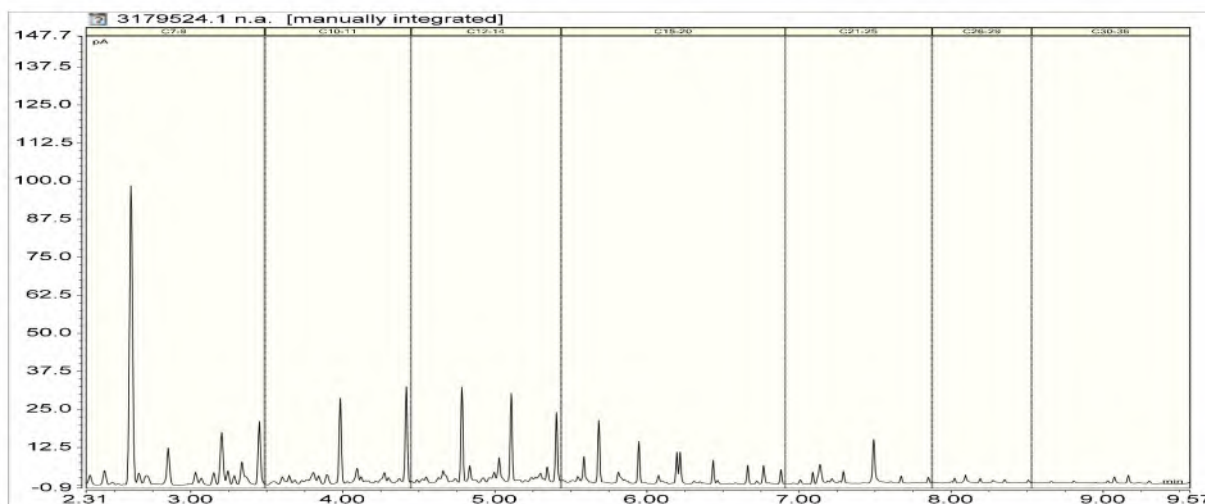

Analyst's Comments

#1 Severe matrix interferences required that a dilution be performed prior to analysis, resulting in a detection limit higher than that normally achieved for the Total Alkalinity analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	1
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	1

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	1
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	1
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	1
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	1
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	1
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	1
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	1
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	1
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	1
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	1
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 25-Feb-2023 and 06-Mar-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3179525	SPV1
Contact:	Fiona Campbell	Date Received:	22-Feb-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	03-Mar-2023	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	258389	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim5 Return HF Fluid Start & Turangi 18 Stim5 Return HF Fluid Middle		
Lab Number:	3179525.3		
Individual Tests			
pH	pH Units		6.6
Total Alkalinity	g/m ³ as CaCO ₃		880
Total Hardness	g/m ³ as CaCO ₃		78
Electrical Conductivity (EC)	mS/m		490
Salinity*			2.6
Total Suspended Solids	g/m ³		260
Total Dissolved Solids (TDS)	g/m ³		4,900
Dissolved Barium	g/m ³		2.0
Dissolved Bromine	g/m ³		3.4
Dissolved Calcium	g/m ³		22
Dissolved Copper	g/m ³		0.010
Dissolved Iron	g/m ³		16.8
Dissolved Magnesium	g/m ³		5
Dissolved Manganese	g/m ³		0.92
Total Nickel*	g/m ³		0.29
Total Potassium*	g/m ³		59
Total Sodium*	g/m ³		1,010
Total Sulphur	g/m ³		13
Total Zinc*	g/m ³		0.057
Chloride	g/m ³		820
Nitrite-N	g/m ³		< 0.10 #2
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #2
Sulphate*	g/m ³		38
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 30 #1
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 110
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		10.4
Toluene	g/m ³		4.1
Ethylbenzene	g/m ³		0.128
m&p-Xylene	g/m ³		0.67
o-Xylene	g/m ³		0.33




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous	
Sample Name:	Composite of Turangi 18 Stim5 Return HF Fluid Start & Turangi 18 Stim5 Return HF Fluid Middle
Lab Number:	3179525.3
Formaldehyde in Water by DNPH & LCMSMS	
Formaldehyde	g/m ³ < 1.5
Total Petroleum Hydrocarbons in Water	
C7 - C9	g/m ³ 20
C10 - C14	g/m ³ 73
C15 - C36	g/m ³ 63
Total hydrocarbons (C7 - C36)	g/m ³ 156

3179525.3

Composite of Turangi 18 Stim5 Return HF Fluid Start & Turangi 18 Stim5 Return HF Fluid Middle

Client Chromatogram for TPH by FID

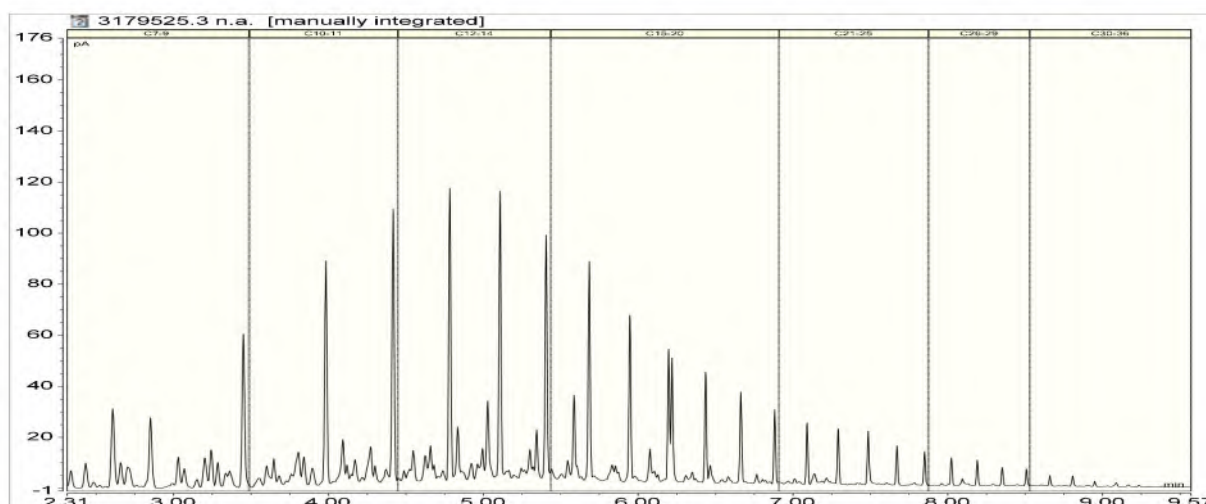

Analyst's Comments

#1 Due to some interference found in the chromatography, the detection limit was raised. Hence the higher detection limit reported.

#2 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	3
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
pH	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	3
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	3

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	3
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	3
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	3
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	3
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	3
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	3
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	3
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	3
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	3
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	3
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	3
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	3
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	3
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	3
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	3
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	3
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	3
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	3
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	3
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	3
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	3
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	3
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	3
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	3
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	3

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 25-Feb-2023 and 03-Mar-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3160153	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	26-Jan-2023	
		Date Reported:	07-Feb-2023	
		Quote No:	81870	
		Order No:	258355	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 4 return HF Fluid		
Lab Number:	3160153.4		
Individual Tests			
pH	pH Units		6.8
Total Alkalinity	g/m ³ as CaCO ₃		900
Total Hardness	g/m ³ as CaCO ₃		290
Electrical Conductivity (EC)	mS/m		1,751
Salinity*			10.9
Total Suspended Solids	g/m ³		220
Total Dissolved Solids (TDS)	g/m ³		13,400
Dissolved Barium	g/m ³		35
Dissolved Bromine	g/m ³		24
Dissolved Calcium	g/m ³		89
Dissolved Copper	g/m ³		0.007
Dissolved Iron	g/m ³		2.1
Dissolved Magnesium	g/m ³		16
Dissolved Manganese	g/m ³		0.44
Total Nickel*	g/m ³		0.092
Total Potassium*	g/m ³		151
Total Sodium*	g/m ³		3,900
Total Sulphur	g/m ³		9
Total Zinc*	g/m ³		0.079
Chloride	g/m ³		5,900
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		28
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		14.0
Toluene	g/m ³		21
Ethylbenzene	g/m ³		1.76
m&p-Xylene	g/m ³		11.7
o-Xylene	g/m ³		3.6




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 4 return HF Fluid	
Lab Number:	3160153.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	193
C10 - C14	g/m ³	360
C15 - C36	g/m ³	440
Total hydrocarbons (C7 - C36)	g/m ³	1,000

3160153.4
 Composite of Turangi 18 Stim 4 return HF Fluid
 Client Chromatogram for TPH by FID

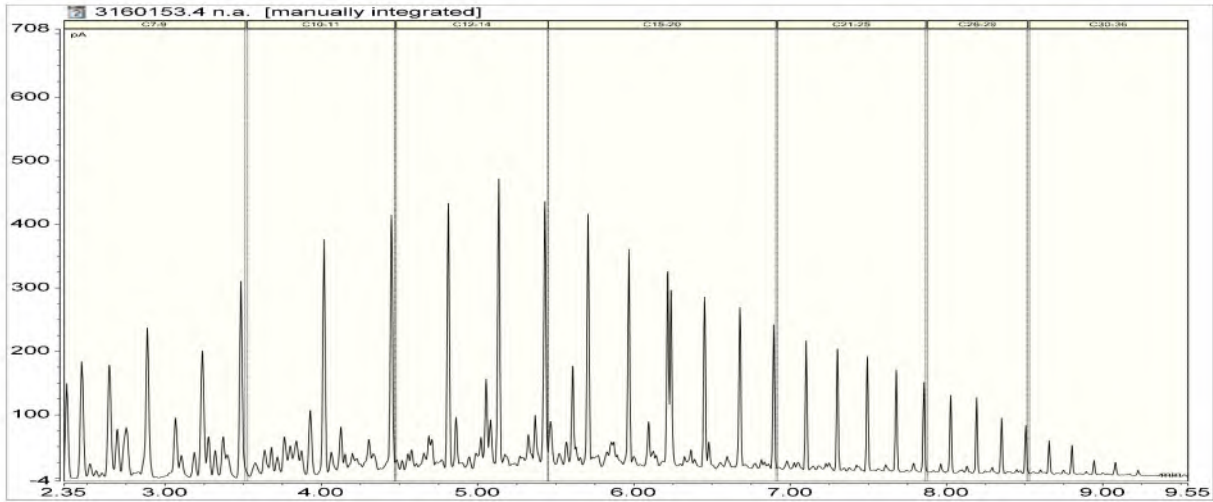

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 28-Jan-2023 and 07-Feb-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, appearing to read 'Graham Corban', is positioned above the printed name.

Graham Corban MSc Tech (Hons)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3160152	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	26-Jan-2023	
		Date Reported:	10-Feb-2023	
		Quote No:	81870	
		Order No:	258259	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 3 Return HF Fluid		
Lab Number:	3160152.3		
Individual Tests			
pH	pH Units		6.6
Total Alkalinity	g/m ³ as CaCO ₃		450
Total Hardness	g/m ³ as CaCO ₃		187
Electrical Conductivity (EC)	mS/m		970
Salinity*			5.5
Total Suspended Solids	g/m ³		770
Total Dissolved Solids (TDS)	g/m ³		8,000
Dissolved Barium	g/m ³		7.4
Dissolved Bromine	g/m ³		9.5
Dissolved Calcium	g/m ³		49
Dissolved Copper	g/m ³		0.34
Dissolved Iron	g/m ³		7.9
Dissolved Magnesium	g/m ³		16
Dissolved Manganese	g/m ³		1.64
Total Nickel*	g/m ³		0.39
Total Potassium*	g/m ³		97
Total Sodium*	g/m ³		1,810
Total Sulphur	g/m ³		< 60
Total Zinc*	g/m ³		0.76
Chloride	g/m ³		2,900
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		0.14
Nitrate	g/m ³		0.6
Nitrate-N + Nitrite-N	g/m ³		0.16 #1
Sulphate*	g/m ³		< 160
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		55
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		17.3
Toluene	g/m ³		44
Ethylbenzene	g/m ³		4.3
m&p-Xylene	g/m ³		30
o-Xylene	g/m ³		9.3




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 3 Return HF Fluid		
Lab Number:	3160152.3		
Formaldehyde in Water by DNPH & LCMSMS			
Formaldehyde	g/m ³	4.0	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	5,700	
C10 - C14	g/m ³	9,300	
C15 - C36	g/m ³	14,400	
Total hydrocarbons (C7 - C36)	g/m ³	29,000	

3160152.3
 Composite of Turangi 18 Stim 3 Return HF Fluid
 Client Chromatogram for TPH by FID

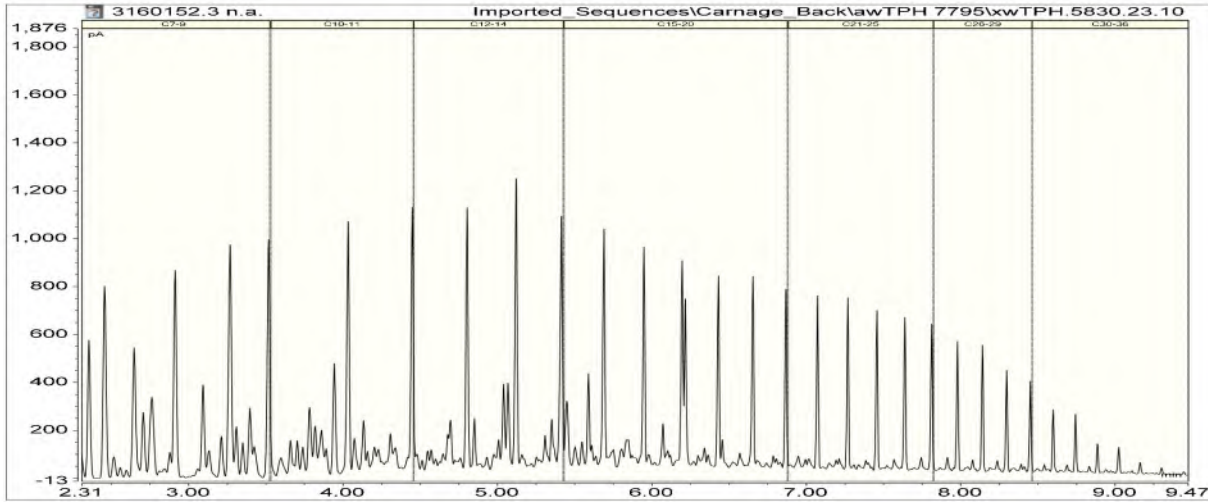

Analyst's Comments

It has been noted that the duplicate for the BTEX analysis on sample 3160152.3, which was run as part of our in-house QC procedure, showed greater variation than would normally be expected. This may reflect the heterogeneity of the sample. The non-aqueous oil phase maybe contributing to the variance observed within the aqueous phase.

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	3
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
pH	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	3
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	3

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	3
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	3
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	3
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	3
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	3
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	3
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	3
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	3
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	3
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	3
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	3
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	3
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	3
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	3
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	3
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	3
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	3
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	3
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	3
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	3
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	3
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	3
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	3
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	3
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	3

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 28-Jan-2023 and 10-Feb-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3140108	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	19-Dec-2022	
		Date Reported:	05-Jan-2023	
		Quote No:	81870	
		Order No:	258013	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 2 Return HF Fluid		
Lab Number:	3140108.4		
Individual Tests			
pH	pH Units		6.7
Total Alkalinity	g/m ³ as CaCO ₃		750
Total Hardness	g/m ³ as CaCO ₃		320
Electrical Conductivity (EC)	mS/m		1,798
Salinity*			10.9
Total Suspended Solids	g/m ³		310
Total Dissolved Solids (TDS)	g/m ³		12,400
Dissolved Barium	g/m ³		54
Dissolved Bromine	g/m ³		15.8
Dissolved Calcium	g/m ³		109
Dissolved Copper	g/m ³		0.067
Dissolved Iron	g/m ³		1.66
Dissolved Magnesium	g/m ³		11
Dissolved Manganese	g/m ³		2.4
Total Nickel*	g/m ³		0.076
Total Potassium*	g/m ³		330
Total Sodium*	g/m ³		3,800
Total Sulphur	g/m ³		8
Total Zinc*	g/m ³		0.080
Chloride	g/m ³		5,900
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		24
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		27
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		33
Toluene	g/m ³		34
Ethylbenzene	g/m ³		2.8
m&p-Xylene	g/m ³		15.6
o-Xylene	g/m ³		4.6




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 2 Return HF Fluid	
Lab Number:	3140108.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	0.59
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	177
C10 - C14	g/m ³	330
C15 - C36	g/m ³	450
Total hydrocarbons (C7 - C36)	g/m ³	960

3140108.4
 Composite of Turangi 18 Stim 2 Return HF Fluid
 Client Chromatogram for TPH by FID

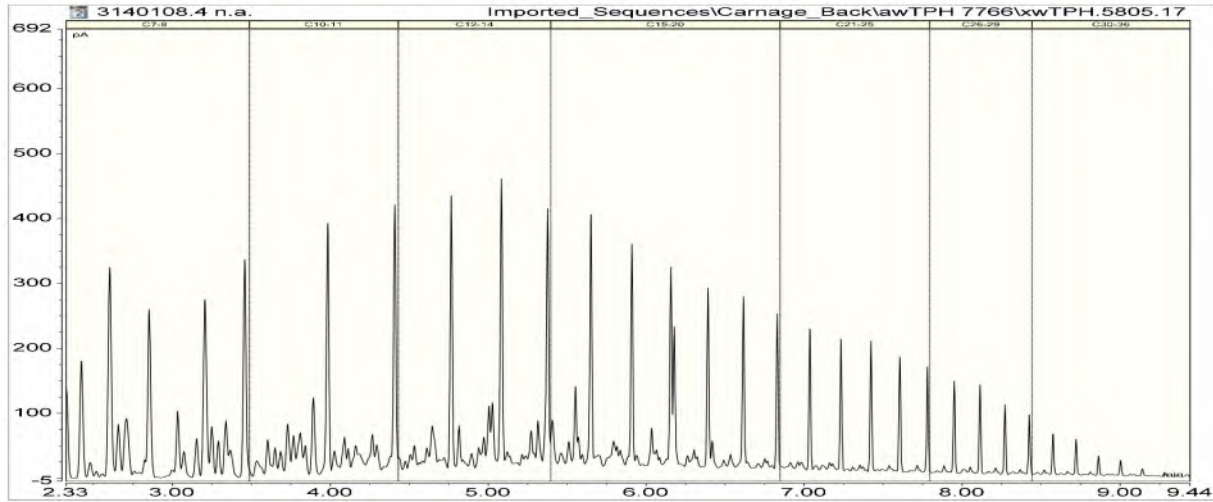**Analyst's Comments**

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Dec-2022 and 05-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, appearing to read 'Graham Corban', is positioned above the printed name.

Graham Corban MSc Tech (Hons)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3140109	SPV1
Contact:	Fiona Campbell	Date Received:	19-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	30-Dec-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	258014	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 1 Return HF Fluid		
Lab Number:	3140109.4		
Individual Tests			
pH	pH Units		6.8
Total Alkalinity	g/m ³ as CaCO ₃		1,330
Total Hardness	g/m ³ as CaCO ₃		131
Electrical Conductivity (EC)	mS/m		775
Salinity*			4.4
Total Suspended Solids	g/m ³		220
Total Dissolved Solids (TDS)	g/m ³		7,000
Dissolved Barium	g/m ³		9.6
Dissolved Bromine	g/m ³		5.3
Dissolved Calcium	g/m ³		43
Dissolved Copper	g/m ³		0.009
Dissolved Iron	g/m ³		4.5
Dissolved Magnesium	g/m ³		6
Dissolved Manganese	g/m ³		1.14
Total Nickel*	g/m ³		0.070
Total Potassium*	g/m ³		64
Total Sodium*	g/m ³		1,760
Total Sulphur	g/m ³		10
Total Zinc*	g/m ³		0.093
Chloride	g/m ³		1,810
Nitrite-N	g/m ³		< 0.10
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10
Sulphate*	g/m ³		31
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		36
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		9.6
Toluene	g/m ³		7.0
Ethylbenzene	g/m ³		0.40
m&p-Xylene	g/m ³		2.2
o-Xylene	g/m ³		0.80




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 18 Stim 1 Return HF Fluid	
Lab Number:	3140109.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	17.0
C10 - C14	g/m ³	45
C15 - C36	g/m ³	104
Total hydrocarbons (C7 - C36)	g/m ³	166

3140109.4
 Composite of Turangi 18 Stim 1 Return HF Fluid
 Client Chromatogram for TPH by FID

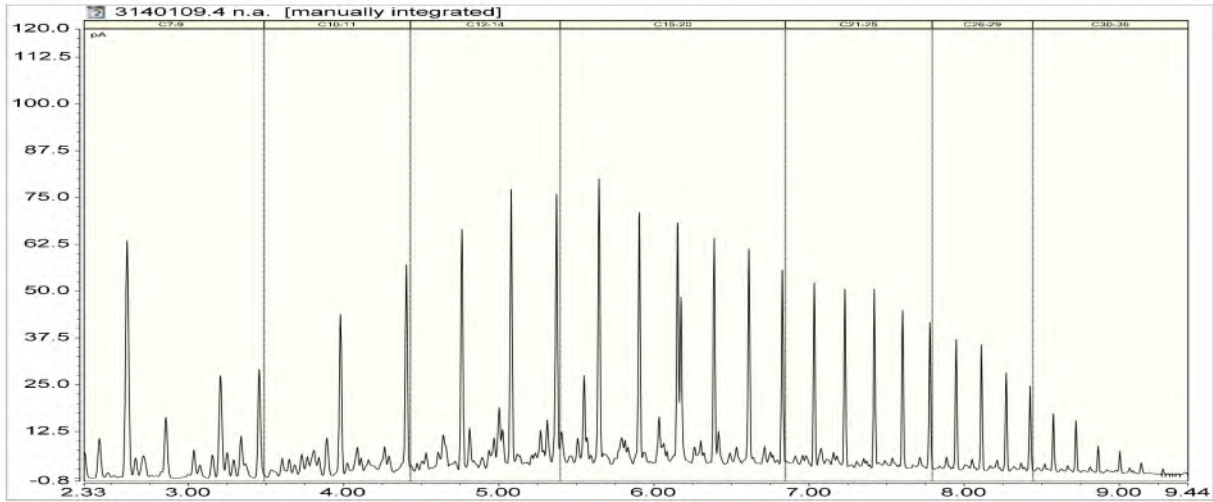

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Dec-2022 and 30-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized lines that form a unique, somewhat abstract shape.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3168120	SPV1
Contact:	Fiona Campbell	Date Received:	08-Feb-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	23-Feb-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258471	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 18 Stim 6 Prepumped HF Fluids 01-Feb-2023		
Lab Number:	3168120.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	109	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	< 0.0010	
Toluene	g/m ³	0.0048	
Ethylbenzene	g/m ³	< 0.0010	
m&p-Xylene	g/m ³	0.005	
o-Xylene	g/m ³	0.0025	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 09-Feb-2023 and 23-Feb-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental




Certificate of Analysis

Client: Greymouth Petroleum Limited	Lab No: 3162753	SPV1
Contact: Fiona Campbell	Date Received: 31-Jan-2023	
C/- Greymouth Petroleum Limited	Date Reported: 14-Feb-2023	
14 Connett Road West	Quote No: 85159	
Bell Block	Order No: 258389	
New Plymouth 4312	Client Reference: Hydraulic fracturing fluid testing	
	Submitted By: Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 18 Stim 5 Prepumped HF Fluid 26-Jan-2023	
Lab Number:	3162753.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	101
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	0.0046
Toluene	g/m ³	0.0167
Ethylbenzene	g/m ³	0.0018
m&p-Xylene	g/m ³	0.015
o-Xylene	g/m ³	0.0057
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	3
Total hydrocarbons (C7 - C36)	g/m ³	< 4

3162753.1
Turangi 18 Stim 5 Prepumped HF Fluid 26-Jan-2023
Client Chromatogram for TPH by FID

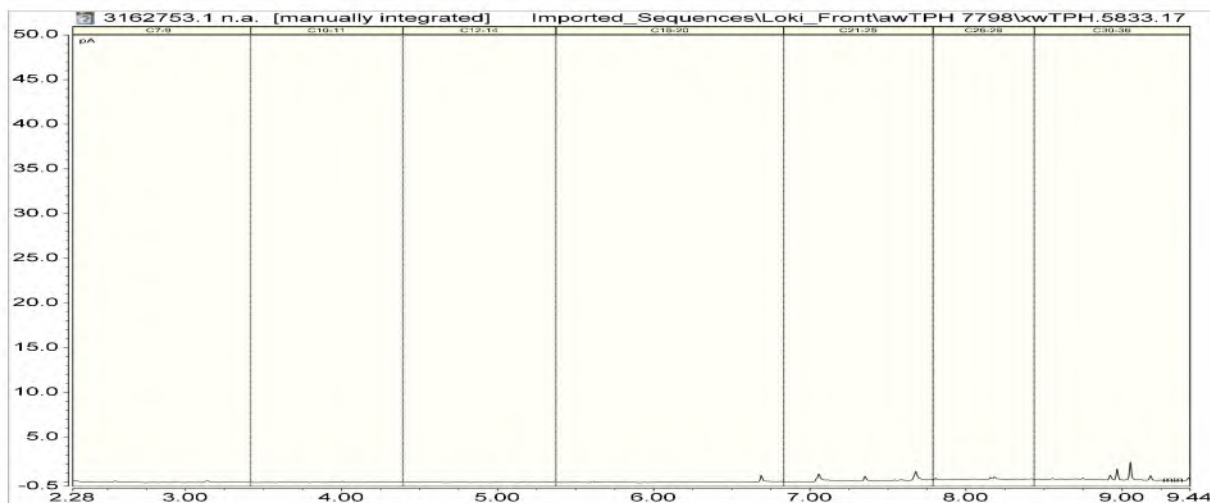

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 03-Feb-2023 and 14-Feb-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3156175	SPV1
Contact:	Fiona Campbell	Date Received:	20-Jan-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	31-Jan-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258355	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 18 Stim 4 Prepumped HF Fluids 18-Jan-2023		
Lab Number:	3156175.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	93	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0026	
Toluene	g/m ³	0.0122	
Ethylbenzene	g/m ³	0.0015	
m&p-Xylene	g/m ³	0.011	
o-Xylene	g/m ³	0.0042	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 23-Jan-2023 and 31-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping loops and lines, positioned above the name of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental




Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3149993	SPV1
Contact:	Fiona Campbell	Date Received:	12-Jan-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	17-Jan-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258259	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 18 Stim3 Prepumped HF Fluid 05-Jan-2023		
Lab Number:	3149993.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	71	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0020	
Toluene	g/m ³	0.0087	
Ethylbenzene	g/m ³	0.0014	
m&p-Xylene	g/m ³	0.009	
o-Xylene	g/m ³	0.0034	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.2	
C10 - C14	g/m ³	< 0.4	
C15 - C36	g/m ³	1.5	
Total hydrocarbons (C7 - C36)	g/m ³	1.5	

3149993.1
Turangi 18 Stim3 Prepumped HF Fluid 05-Jan-2023
Client Chromatogram for TPH by FID

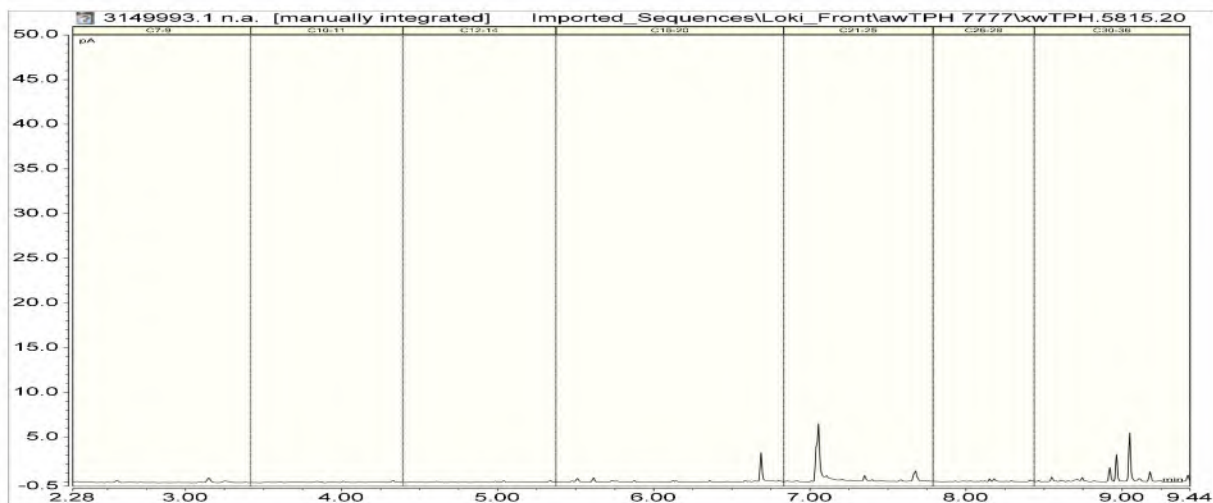

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-Jan-2023 and 17-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Graham Corban MSc Tech (Hons)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3139752	SPV1
Contact:	Fiona Campbell	Date Received:	17-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	22-Dec-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258013	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 18 Stim 2 Prepumped HF Fluid 12-Dec-2022		
Lab Number:	3139752.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	109	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0020	
Toluene	g/m ³	0.0129	
Ethylbenzene	g/m ³	0.0018	
m&p-Xylene	g/m ³	0.014	
o-Xylene	g/m ³	0.0052	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 20-Dec-2022 and 22-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental




Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3134636	SPv2
Contact:	Fiona Campbell	Date Received:	10-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	27-Jan-2023	(Amended)
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258014	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi 18 Stim #1 Prepumped HF Fluid 05-Dec-2022	
Lab Number:	3134636.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	820
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	0.0035
Toluene	g/m ³	0.020
Ethylbenzene	g/m ³	0.0027
m&p-Xylene	g/m ³	0.018
o-Xylene	g/m ³	0.0070
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.5
C10 - C14	g/m ³	< 1.0
C15 - C36	g/m ³	3
Total hydrocarbons (C7 - C36)	g/m ³	< 4

3134636.1
Turangi 18 Stim #1 Prepumped HF Fluid 05-Dec-2022
Client Chromatogram for TPH by FID

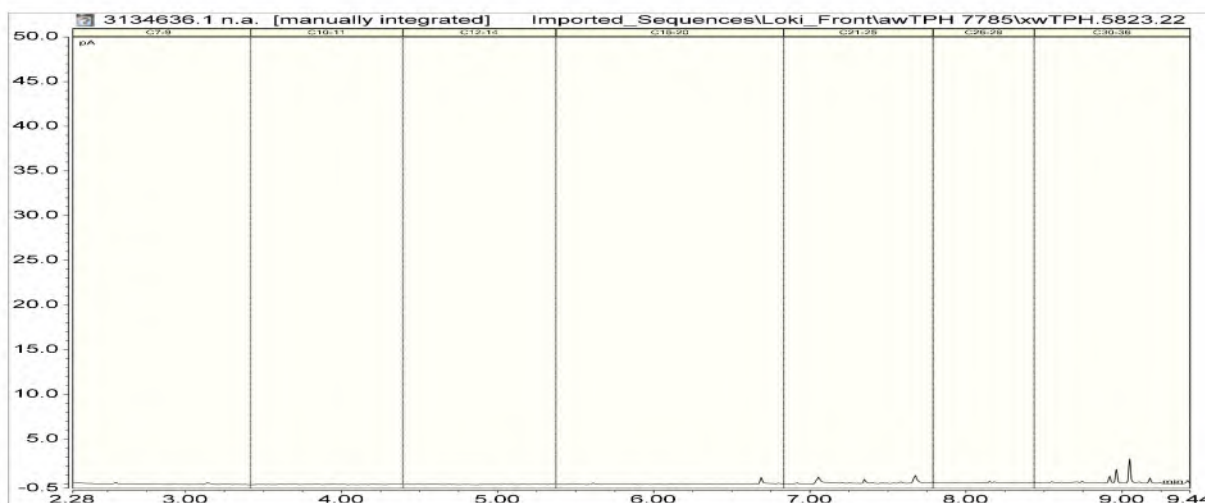

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Analyst's Comments

Amended Report: This certificate of analysis replaces report '3134636-SPv1' issued on 22-Dec-2022 at 4:32 pm. Reason for amendment: As part of a Quality of Work Query (89956), the TPH was repeated and the repeat result for this analysis has now been reported.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 13-Dec-2022 and 24-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3000886	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	28-May-2022	
		Date Reported:	10-Jun-2022	
		Quote No:	81870	
		Order No:	255994	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 16 Stim #7 Return HF Fluid START 19-May-2022				
Lab Number:	3000886.1				

Individual Tests						
pH*	pH Units	6.8	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	102	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	89	-	-	-	-
Electrical Conductivity (EC)*	mS/m	90.4	-	-	-	-
Salinity*		0.2	-	-	-	-
Total Suspended Solids	g/m ³	1,040	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	3,300	-	-	-	-
Dissolved Barium	g/m ³	0.106	-	-	-	-
Dissolved Bromine	g/m ³	< 0.5	-	-	-	-
Dissolved Calcium	g/m ³	24	-	-	-	-
Dissolved Copper	g/m ³	0.092	-	-	-	-
Dissolved Iron	g/m ³	2.9	-	-	-	-
Dissolved Magnesium	g/m ³	7	-	-	-	-
Dissolved Manganese	g/m ³	0.124	-	-	-	-
Total Nickel	g/m ³	0.35	-	-	-	-
Total Potassium	g/m ³	13.0	-	-	-	-
Total Sodium	g/m ³	63	-	-	-	-
Total Sulphur*	g/m ³	12	-	-	-	-
Total Zinc	g/m ³	0.56	-	-	-	-
Chloride*	g/m ³	240	-	-	-	-
Nitrite-N	g/m ³	< 0.10 #3	-	-	-	-
Nitrate-N	g/m ³	< 0.10	-	-	-	-
Nitrate*	g/m ³	< 0.5	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #3	-	-	-	-
Sulphate*	g/m ³	36	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	220	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	52	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:	Turangi 16 Stim #7 Return HF Fluid START 19-May-2022				
Lab Number:	3000886.1				

BTEX in Water by Headspace GC-MS*

Benzene*	g/m ³	660 #2	-	-	-	-
Toluene*	g/m ³	1,630 #2	-	-	-	-
Ethylbenzene*	g/m ³	330 #2	-	-	-	-
m&p-Xylene*	g/m ³	1,220 #2	-	-	-	-
o-Xylene*	g/m ³	570 #2	-	-	-	-


Formaldehyde in Water by DNPH & LCMSMS*

Formaldehyde*	g/m ³	1.7	-	-	-	-
---------------	------------------	-----	---	---	---	---

Total Petroleum Hydrocarbons in Water*

C7 - C9*	g/m ³	1,450 #1	-	-	-	-
C10 - C14*	g/m ³	1,260	-	-	-	-
C15 - C36*	g/m ³	660	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	3,400	-	-	-	-

3000886.1
Turangi 16 Stim #7 Return HF Fluid START 19-May-2022
Client Chromatogram for TPH by FID

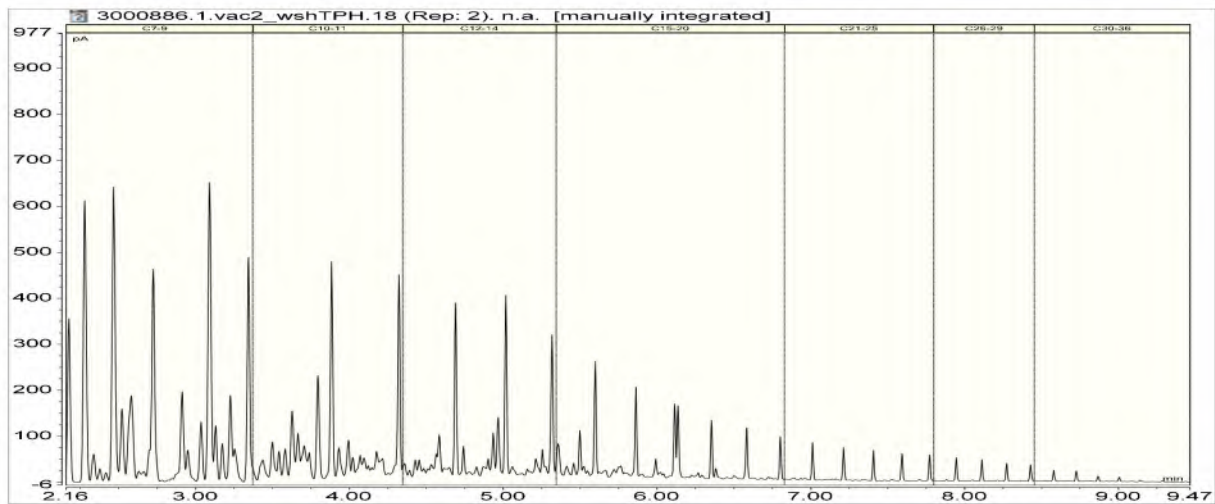

Analyst's Comments

- #1 It was observed that the BTEX was greater than the C7-C9. Both analyses were repeated and the same pattern has occurred, indicating the sample is inhomogenous and there is a possible difference in the bottles supplied.
- #2 The dilution results for the BTEX analysis showed greater variation than what would be expected. The dilution was repeated and the same issue occurred, indicating the sample is inhomogenous. Results have been averaged.
- #3 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	1
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
pH*	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	1
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	1
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	1
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	1
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	1
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	1
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	1
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	1
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	1
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	1
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	1
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	1
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Total Petroleum Hydrocarbons in Water			

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 31-May-2022 and 10-Jun-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Carole Rodgers-Carroll BA, NZCS
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3000885	SPV1
Contact:	Fiona Campbell	Date Received:	28-May-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	15-Jun-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	255911	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 16 Stim #6 Return HF Fluid START 11-May-2022				
Lab Number:	3000885.1				

Individual Tests

pH*	pH Units	5.1	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	153	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	101	-	-	-	-
Electrical Conductivity (EC)*	mS/m	161.2	-	-	-	-
Salinity*		0.6	-	-	-	-
Total Suspended Solids	g/m ³	220	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	3,200	-	-	-	-
Dissolved Barium	g/m ³	1.33	-	-	-	-
Dissolved Bromine	g/m ³	0.9	-	-	-	-
Dissolved Calcium	g/m ³	28	-	-	-	-
Dissolved Copper	g/m ³	0.068	-	-	-	-
Dissolved Iron	g/m ³	6.0	-	-	-	-
Dissolved Magnesium	g/m ³	8	-	-	-	-
Dissolved Manganese	g/m ³	0.156	-	-	-	-
Total Nickel	g/m ³	1.06	-	-	-	-
Total Potassium	g/m ³	17.3	-	-	-	-
Total Sodium	g/m ³	210	-	-	-	-
Total Sulphur*	g/m ³	16.5	-	-	-	-
Total Zinc	g/m ³	0.158	-	-	-	-
Chloride*	g/m ³	360	-	-	-	-
Nitrite-N	g/m ³	< 0.10 #1	-	-	-	-
Nitrate-N	g/m ³	< 0.10	-	-	-	-
Nitrate*	g/m ³	< 0.5	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #2	-	-	-	-
Sulphate*	g/m ³	49	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	164	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:	Turangi 16 Stim #6 Return HF Fluid START 11-May-2022					
Lab Number:	3000885.1					
BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	19.5	-	-	-	-
Toluene*	g/m ³	20	-	-	-	-
Ethylbenzene*	g/m ³	1.83	-	-	-	-
m&p-Xylene*	g/m ³	11.0	-	-	-	-
o-Xylene*	g/m ³	3.8	-	-	-	-
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	< 0.15	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	90	-	-	-	-
C10 - C14*	g/m ³	192	-	-	-	-
C15 - C36*	g/m ³	250	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	530	-	-	-	-

3000885.1
Turangi 16 Stim #6 Return HF Fluid START 11-May-2022
Client Chromatogram for TPH by FID

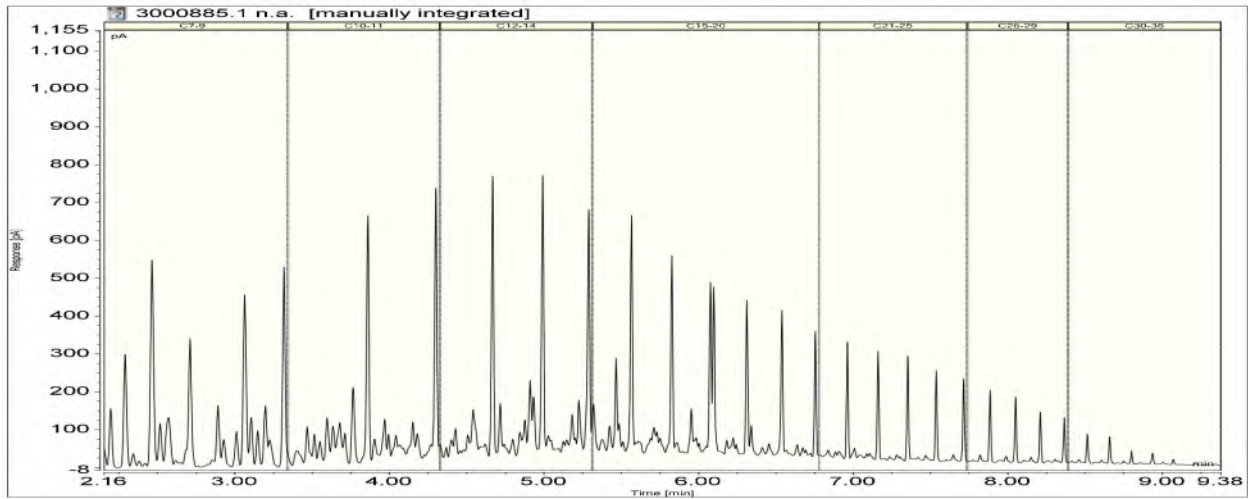

Analyst's Comments

- #1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N analysis.
- #2 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO_xN analysis.

Summary of Methods

The following table(s) give a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	1
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	1

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
pH*	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	1
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	1
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	1
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	1
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	1
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	1
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	1
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	1
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	1
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	1
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	1
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	1
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	1
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	1
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	1
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	1
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	1
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	1
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	1
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	1
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	1
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	1
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	1
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	1
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	1
Total Petroleum Hydrocarbons in Water			

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 30-May-2022 and 10-Jun-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Carole Rodgers-Carroll BA, NZCS
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	2990452	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	18-May-2022	
		Date Reported:	30-May-2022	
		Quote No:	81870	
		Order No:	255730	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 16 Stim 5 return HF Fluid				
Lab Number:	2990452.3				
Individual Tests					
pH*	pH Units	7.3	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	1,670	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	139	-	-	-
Electrical Conductivity (EC)*	mS/m	976	-	-	-
Salinity*		5.6	-	-	-
Total Suspended Solids	g/m ³	680	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	7,600	-	-	-
Dissolved Barium	g/m ³	11.6	-	-	-
Dissolved Bromine	g/m ³	8.6	-	-	-
Dissolved Calcium	g/m ³	41	-	-	-
Dissolved Copper	g/m ³	0.020	-	-	-
Dissolved Iron	g/m ³	2.5	-	-	-
Dissolved Magnesium	g/m ³	9	-	-	-
Dissolved Manganese	g/m ³	0.73	-	-	-
Total Nickel	g/m ³	0.167	-	-	-
Total Potassium	g/m ³	73	-	-	-
Total Sodium	g/m ³	2,300	-	-	-
Total Sulphur*	g/m ³	12	-	-	-
Total Zinc	g/m ³	0.43	-	-	-
Chloride*	g/m ³	2,300	-	-	-
Nitrite-N	g/m ³	< 0.010 #1	-	-	-
Nitrate-N	g/m ³	< 0.010	-	-	-
Nitrate*	g/m ³	< 0.05	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.010 #1	-	-	-
Sulphate*	g/m ³	37	-	-	-
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	< 20	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS*					
Benzene*	g/m ³	85	-	-	-
Toluene*	g/m ³	55	-	-	-
Ethylbenzene*	g/m ³	2.5	-	-	-
m&p-Xylene*	g/m ³	16.3	-	-	-
o-Xylene*	g/m ³	4.7	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name: Turangi 16 Stim 5 return HF Fluid					
Lab Number: 2990452.3					
Formaldehyde in Water by DNPH & LCMSMS*					
Formaldehyde*	g/m ³	< 1.5	-	-	-
Total Petroleum Hydrocarbons in Water*					
C7 - C9*	g/m ³	172	-	-	-
C10 - C14*	g/m ³	146	-	-	-
C15 - C36*	g/m ³	122	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	440	-	-	-

2990452.3
 Turangi 16 Stim 5 return HF Fluid
 Client Chromatogram for TPH by FID

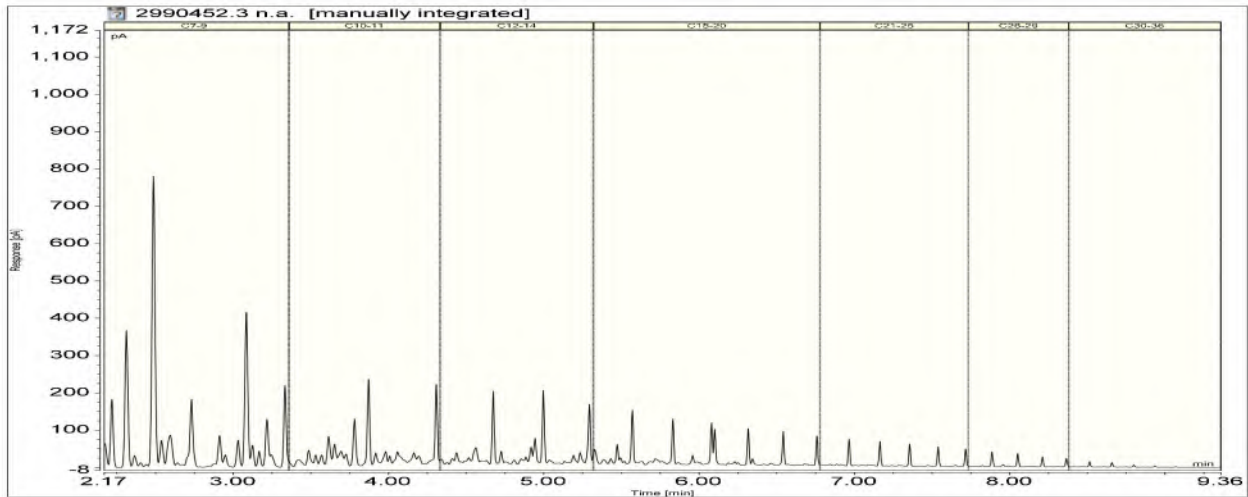

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	3
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	3
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	3
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	3
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	3

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	3
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	3
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	3
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	3
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	3
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	3
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	3
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	3
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	3
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	3
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	3
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	3
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	3
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	3
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	3
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	3
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	3
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	3
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	3
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	3
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	3
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	3
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	3
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	3

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 19-May-2022 and 30-May-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2967653	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	27-Apr-2022	
		Date Reported:	05-May-2022	
		Quote No:	81870	
		Order No:	255672	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Composite of Turangi 16 Stim 4 return HF Fluid Start, Turangi 16 Stim 4 return HF Fluid Middle and Turangi 16 Stim 4 return HF Fluid End				
Lab Number:	2967653.4				

Individual Tests						
pH*	pH Units	6.3	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	780	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	270	-	-	-	-
Electrical Conductivity (EC)*	mS/m	1,540	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	10,200	-	-	-	-
Dissolved Barium	g/m ³	23	-	-	-	-
Dissolved Bromine	g/m ³	19.1	-	-	-	-
Dissolved Calcium	g/m ³	84	-	-	-	-
Dissolved Copper	g/m ³	0.026	-	-	-	-
Dissolved Iron	g/m ³	5.9	-	-	-	-
Dissolved Magnesium	g/m ³	14	-	-	-	-
Dissolved Manganese	g/m ³	0.52	-	-	-	-
Total Nickel	g/m ³	< 0.032	-	-	-	-
Total Potassium	g/m ³	104	-	-	-	-
Total Sodium	g/m ³	3,300	-	-	-	-
Total Sulphur*	g/m ³	9.4	-	-	-	-
Total Zinc	g/m ³	0.144	-	-	-	-
Chloride*	g/m ³	4,600	-	-	-	-
Nitrite-N	g/m ³	< 0.0010	-	-	-	-
Nitrate-N	g/m ³	< 0.0010	-	-	-	-
Nitrate*	g/m ³	< 0.005	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.0010	-	-	-	-
Sulphate*	g/m ³	28	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	74	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.


Sample Type: Saline

Sample Name:	Composite of Turangi 16 Stim 4 return HF Fluid Start, Turangi 16 Stim 4 return HF Fluid Middle and Turangi 16 Stim 4 return HF Fluid End				
Lab Number:	2967653.4				

BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	74	-	-	-	-
Toluene*	g/m ³	107	-	-	-	-
Ethylbenzene*	g/m ³	11.1	-	-	-	-
m&p-Xylene*	g/m ³	67	-	-	-	-
o-Xylene*	g/m ³	19.7	-	-	-	-
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	0.26	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	410	-	-	-	-
C10 - C14*	g/m ³	470	-	-	-	-
C15 - C36*	g/m ³	330	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	1,210	-	-	-	-

2967653.4

Composite of Turangi 16 Stim 4 return HF Fluid Start, Turangi 16 Stim 4 return HF Fluid Middle and Turangi 16 Stim 4 return HF Fluid End
Client Chromatogram for TPH by FID

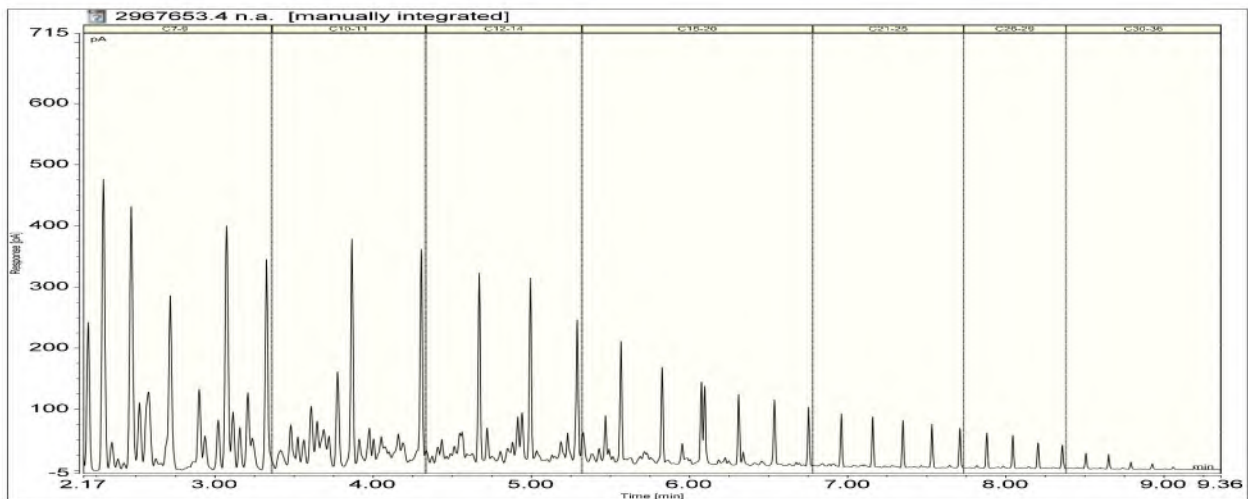

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 30-Apr-2022 and 05-May-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2967655	SPV1
Contact:	Fiona Campbell	Date Received:	27-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	05-May-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	255603	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Composite of Turangi 16 Stim 3 return HF Fluid Start, Turangi 16 Stim 3 return HF Fluid Middle and Turangi 16 Stim 3 return HF Fluid End				
Lab Number:	2967655.4				

Individual Tests						
pH*	pH Units	5.9	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	440	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	430	-	-	-	-
Electrical Conductivity (EC)*	mS/m	1,839	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	15,300	-	-	-	-
Dissolved Barium	g/m ³	43	-	-	-	-
Dissolved Bromine	g/m ³	19.4	-	-	-	-
Dissolved Calcium	g/m ³	152	-	-	-	-
Dissolved Copper	g/m ³	0.007	-	-	-	-
Dissolved Iron	g/m ³	4.5	-	-	-	-
Dissolved Magnesium	g/m ³	13	-	-	-	-
Dissolved Manganese	g/m ³	3.7	-	-	-	-
Total Nickel	g/m ³	0.037	-	-	-	-
Total Potassium	g/m ³	141	-	-	-	-
Total Sodium	g/m ³	3,800	-	-	-	-
Total Sulphur*	g/m ³	7.6	-	-	-	-
Total Zinc	g/m ³	0.082	-	-	-	-
Chloride*	g/m ³	5,800	-	-	-	-
Nitrite-N	g/m ³	< 0.0010	-	-	-	-
Nitrate-N	g/m ³	< 0.0010	-	-	-	-
Nitrate*	g/m ³	< 0.005	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.0010	-	-	-	-
Sulphate*	g/m ³	23	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 20	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:	Composite of Turangi 16 Stim 3 return HF Fluid Start, Turangi 16 Stim 3 return HF Fluid Middle and Turangi 16 Stim 3 return HF Fluid End				
Lab Number:	2967655.4				

BTEX in Water by Headspace GC-MS*

Benzene*	g/m ³	7.7	-	-	-	-
Toluene*	g/m ³	4.0	-	-	-	-
Ethylbenzene*	g/m ³	0.168	-	-	-	-
m&p-Xylene*	g/m ³	0.77	-	-	-	-
o-Xylene*	g/m ³	0.38	-	-	-	-

Formaldehyde in Water by DNPH & LCMSMS*


Formaldehyde*	g/m ³	< 0.15	-	-	-	-
---------------	------------------	--------	---	---	---	---

Total Petroleum Hydrocarbons in Water*

C7 - C9*	g/m ³	4.4	-	-	-	-
C10 - C14*	g/m ³	6.1	-	-	-	-
C15 - C36*	g/m ³	11.7	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	22	-	-	-	-

2967655.4

Composite of Turangi 16 Stim 3 return HF Fluid Start, Turangi 16 Stim 3 return HF Fluid Middle and Turangi 16 Stim 3 return HF Fluid End
Client Chromatogram for TPH by FID

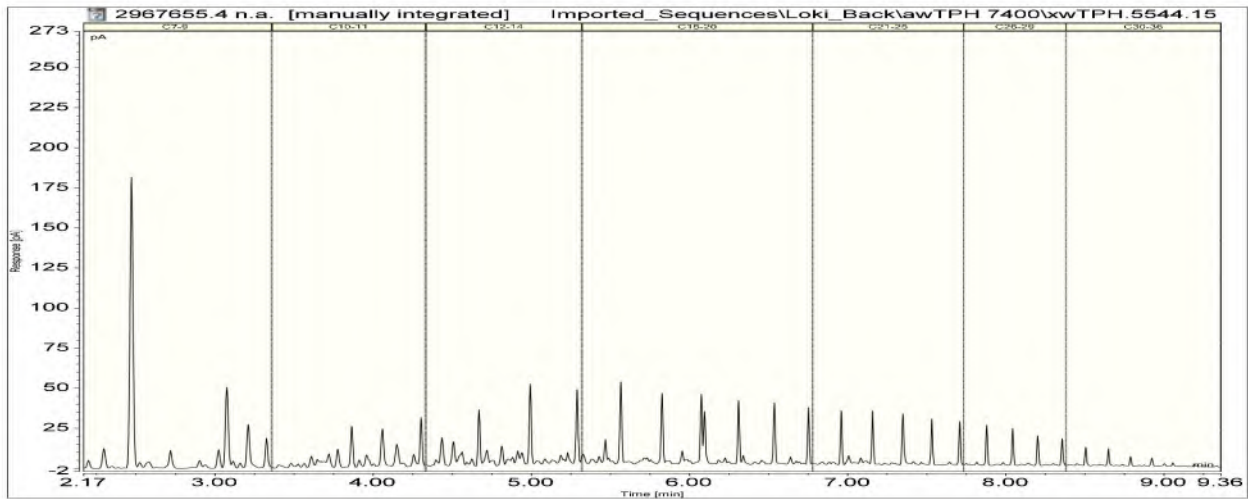

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 30-Apr-2022 and 05-May-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	2946358	SPV1
Contact:	Fiona Campbell	Date Received:	06-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	19-Apr-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	255522	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 16 Stim 2 Return HF Fluid				
Lab Number:	2946358.4				

Individual Tests

pH*	pH Units	6.8	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	670	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	230	-	-	-	-
Electrical Conductivity (EC)*	mS/m	1,253	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	10,000	-	-	-	-
Dissolved Barium	g/m ³	3.6	-	-	-	-
Dissolved Bromine	g/m ³	13.1	-	-	-	-
Dissolved Calcium	g/m ³	75	-	-	-	-
Dissolved Copper	g/m ³	0.012	-	-	-	-
Dissolved Iron	g/m ³	3.3	-	-	-	-
Dissolved Magnesium	g/m ³	11	-	-	-	-
Dissolved Manganese	g/m ³	2.4	-	-	-	-
Total Nickel	g/m ³	0.038 #1	-	-	-	-
Total Potassium	g/m ³	104	-	-	-	-
Total Sodium	g/m ³	2,600	-	-	-	-
Total Sulphur*	g/m ³	14	-	-	-	-
Total Zinc	g/m ³	0.068	-	-	-	-
Chloride*	g/m ³	3,700	-	-	-	-
Nitrite-N	g/m ³	< 0.010 #2	-	-	-	-
Nitrate-N	g/m ³	< 0.010	-	-	-	-
Nitrate*	g/m ³	< 0.05	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.010 #2	-	-	-	-
Sulphate*	g/m ³	41	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 20	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	80	-	-	-	-
BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	9.0	-	-	-	-
Toluene*	g/m ³	4.9	-	-	-	-
Ethylbenzene*	g/m ³	0.186	-	-	-	-
m&p-Xylene*	g/m ³	0.85	-	-	-	-
o-Xylene*	g/m ³	0.36	-	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:		Turangi 16 Stim 2 Return HF Fluid				
Lab Number:		2946358.4				
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	0.23	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	18.8	-	-	-	-
C10 - C14*	g/m ³	36	-	-	-	-
C15 - C36*	g/m ³	79	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	134	-	-	-	-

2946358.4
Turangi 16 Stim 2 Return HF Fluid
Client Chromatogram for TPH by FID

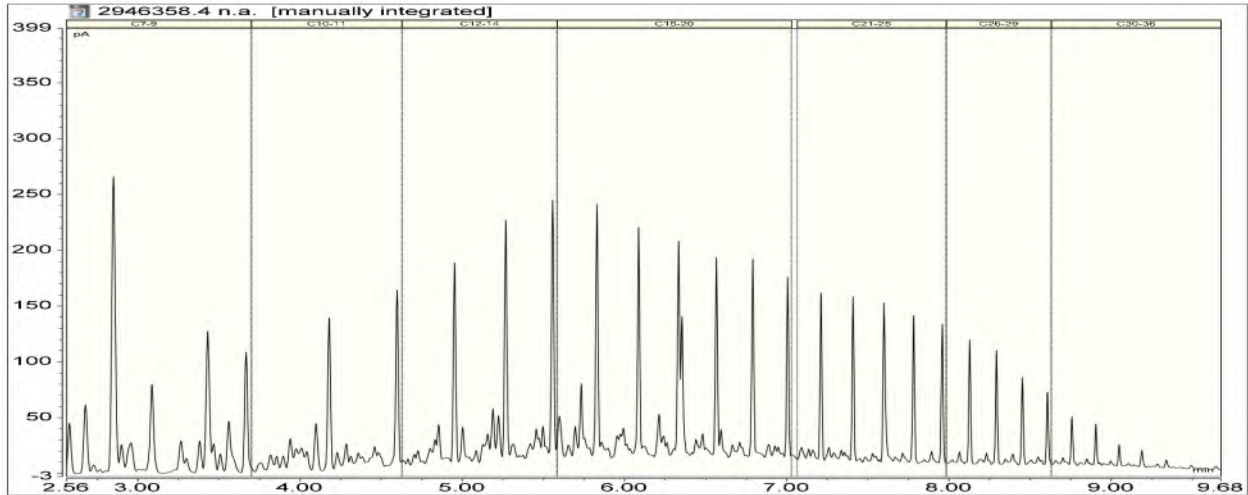

Analyst's Comments

#1 It should be noted that the replicate analyses performed on this sample as part of our in-house Quality Assurance procedures showed greater variation than would normally be expected. This may reflect the heterogeneity of the sample. The average of the results of the replicate analyses has been reported.

#2 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 08-Apr-2022 and 19-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	2946356	SPV1
Contact:	Fiona Campbell	Date Received:	06-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	19-Apr-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	255447	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 16 Stim 7 Return HF			
Lab Number:	2946356.3			

Individual Tests

pH*	pH Units	6.5	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	400	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	160	-	-	-	-
Electrical Conductivity (EC)*	mS/m	565	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	5,400	-	-	-	-
Dissolved Barium	g/m ³	3.6	-	-	-	-
Dissolved Bromine	g/m ³	5.7	-	-	-	-
Dissolved Calcium	g/m ³	53	-	-	-	-
Dissolved Copper	g/m ³	0.059	-	-	-	-
Dissolved Iron	g/m ³	5.0	-	-	-	-
Dissolved Magnesium	g/m ³	7	-	-	-	-
Dissolved Manganese	g/m ³	1.80	-	-	-	-
Total Nickel	g/m ³	0.186 #1	-	-	-	-
Total Potassium	g/m ³	40	-	-	-	-
Total Sodium	g/m ³	1,090	-	-	-	-
Total Sulphur*	g/m ³	16	-	-	-	-
Total Zinc	g/m ³	0.077	-	-	-	-
Chloride*	g/m ³	1,450	-	-	-	-
Nitrite-N	g/m ³	< 0.010 #2	-	-	-	-
Nitrate-N	g/m ³	< 0.010	-	-	-	-
Nitrate*	g/m ³	< 0.05	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	< 0.010 #2	-	-	-	-
Sulphate*	g/m ³	48	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 20	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-
BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	3.5	-	-	-	-
Toluene*	g/m ³	1.09	-	-	-	-
Ethylbenzene*	g/m ³	0.025	-	-	-	-
m&p-Xylene*	g/m ³	0.115	-	-	-	-
o-Xylene*	g/m ³	0.073	-	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:	Turangi 16 Stim 7 Return HF				
Lab Number:	2946356.3				
Formaldehyde in Water by DNPH & LCMSMS*					
Formaldehyde*	g/m ³	< 0.15	-	-	-
Total Petroleum Hydrocarbons in Water*					
C7 - C9*	g/m ³	4.0	-	-	-
C10 - C14*	g/m ³	13.5	-	-	-
C15 - C36*	g/m ³	69	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	87	-	-	-

2946356.3
Turangi 16 Stim 7 Return HF
Client Chromatogram for TPH by FID

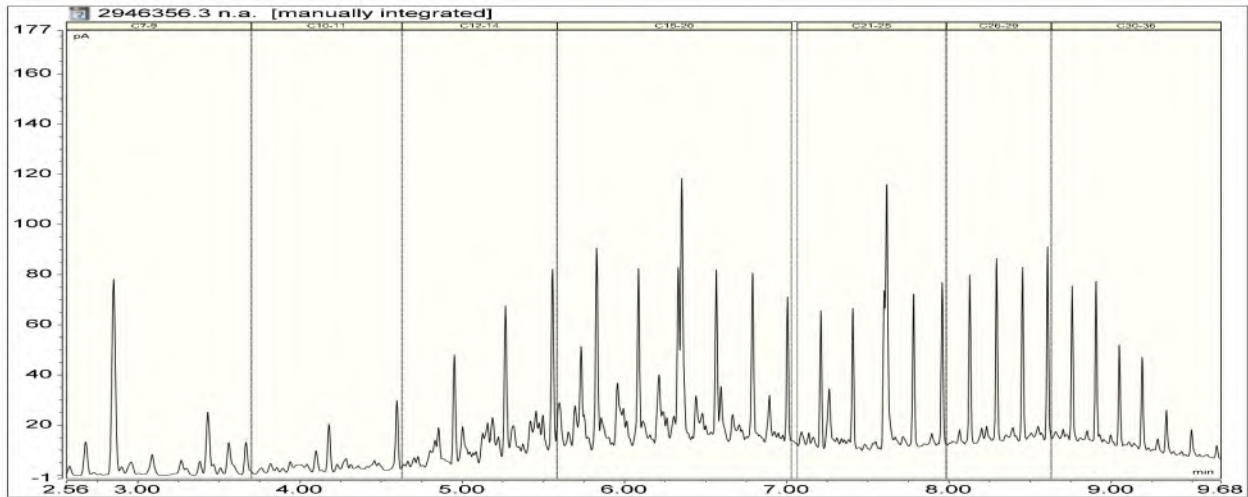

Analyst's Comments

#1 It should be noted that the replicate analyses performed on this sample as part of our in-house Quality Assurance procedures showed greater variation than would normally be expected. This may reflect the heterogeneity of the sample. The average of the results of the replicate analyses has been reported.

#2 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	3
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	3
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	3
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	3

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	3
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	3
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	3
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	3
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	3
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	3
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	3
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	3
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	3
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	3
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	3
Total Zinc	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	3
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	3
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	3
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	3
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	3
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	3
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	3
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	3
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	3
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	3
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	3
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	3

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 08-Apr-2022 and 19-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	2997027	SPV1
Contact:	Fiona Campbell	Date Received:	25-May-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	03-Jun-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255994	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stim #7 Prepumped HF Fluid				
	12-May-2022				
Lab Number:	2997027.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	650	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	< 0.0010	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.4	-	-	-
C10 - C14	g/m ³	< 1.0	-	-	-
C15 - C36	g/m ³	< 2	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 26-May-2022 and 03-Jun-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2985978	SPV1
Contact:	Fiona Campbell	Date Received:	13-May-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	25-May-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255911	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stm #6 Prepumped HF Fluid				
	11-May-2022				
Lab Number:	2985978.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	650	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	< 0.0010	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.15	-	-	-
C10 - C14	g/m ³	< 0.4	-	-	-
C15 - C36	g/m ³	< 0.8	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 1.4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-May-2022 and 25-May-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	2978822	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	06-May-2022	
		Date Reported:	19-May-2022	
		Quote No:	85159	
		Order No:	255730	
		Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stim 5 Prepumped HF Fluid 03-May-2022				
Lab Number:	2978822.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	570	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	0.0016	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.15	-	-	-
C10 - C14	g/m ³	< 0.4	-	-	-
C15 - C36	g/m ³	< 0.8	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 1.4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 11-May-2022 and 19-May-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2958524	SPV1
Contact:	Fiona Campbell	Date Received:	16-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	29-Apr-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255672	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stim 4 Prepumped HF Fluid 12-Apr-2022				
Lab Number:	2958524.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	760	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 400	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	0.0021	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.4	-	-	-
C10 - C14	g/m ³	< 1.0	-	-	-
C15 - C36	g/m ³	< 2	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Apr-2022 and 29-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2951090	SPV1
Contact:	Fiona Campbell	Date Received:	09-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	27-Apr-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255603	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stim3 Prepumped HF Fluid 06-Apr-2022				
Lab Number:	2951090.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	800	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 400	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	0.0025	-	-	-
Toluene	g/m ³	0.0070	-	-	-
Ethylbenzene	g/m ³	0.0011	-	-	-
m&p-Xylene	g/m ³	0.004	-	-	-
o-Xylene	g/m ³	0.0015	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.4	-	-	-
C10 - C14	g/m ³	< 1.0	-	-	-
C15 - C36	g/m ³	< 2	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 12-Apr-2022 and 27-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2944779	SPV1
Contact:	Fiona Campbell	Date Received:	05-Apr-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	21-Apr-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255522	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	


Sample Type: Aqueous

Sample Name:	Turangi 16 Stim 2 prepumped HF Fluid 30-Mar-2022				
Lab Number:	2944779.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	460	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	0.0096	-	-	-
Toluene	g/m ³	0.0174	-	-	-
Ethylbenzene	g/m ³	0.0015	-	-	-
m&p-Xylene	g/m ³	0.007	-	-	-
o-Xylene	g/m ³	0.0029	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.4	-	-	-
C10 - C14	g/m ³	< 1.0	-	-	-
C15 - C36	g/m ³	15	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	16	-	-	-

2944779.1

Turangi 16 Stim 2 prepumped HF Fluid 30-Mar-2022

Client Chromatogram for TPH by FID

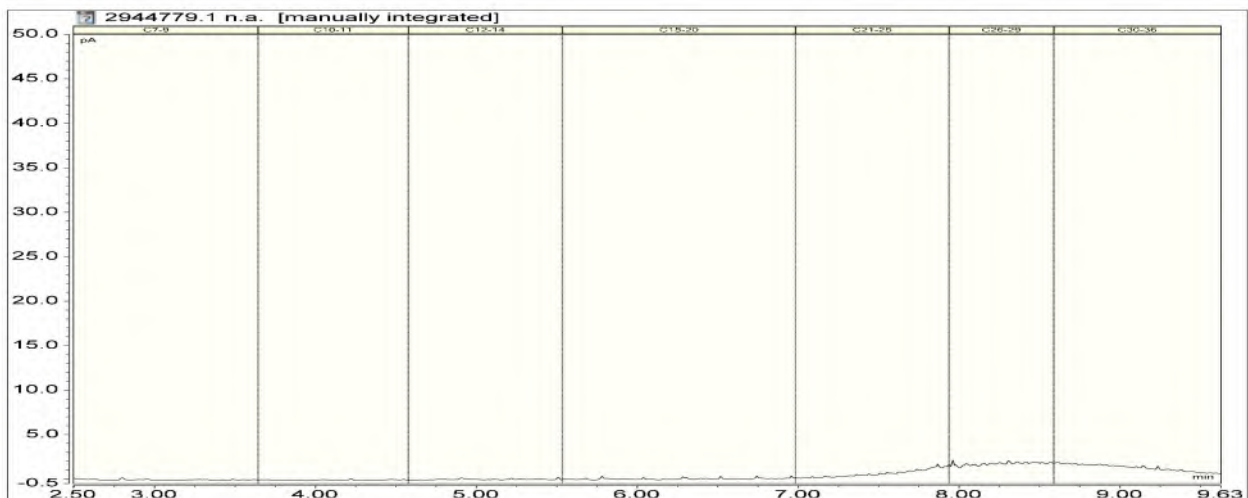

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 11-Apr-2022 and 21-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Kim Harrison MSc
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2937154	SPV1
Contact:	Fiona Campbell	Date Received:	30-Mar-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	08-Apr-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	255447	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 16 Stim 1 Prepumped HF Fluid 24-Mar-2022				
Lab Number:	2937154.1				
Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	1,080	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	< 0.0010	-	-	-
Toluene	g/m ³	0.0023	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	< 0.15	-	-	-
C10 - C14	g/m ³	< 0.4	-	-	-
C15 - C36	g/m ³	< 0.8	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	< 1.4	-	-	-

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 01-Apr-2022 and 08-Apr-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3152661	SPV1
Contact:	Fiona Campbell	Date Received:	17-Jan-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	24-Jan-2023	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	258260	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 7 return HF Fluid		
Lab Number:	3152661.4		
Individual Tests			
pH	pH Units		6.8
Total Alkalinity	g/m ³ as CaCO ₃		840
Total Hardness	g/m ³ as CaCO ₃		97
Electrical Conductivity (EC)	mS/m		396
Salinity*			2.0
Total Suspended Solids	g/m ³		129
Total Dissolved Solids (TDS)	g/m ³		3,600
Dissolved Barium	g/m ³		3.3
Dissolved Bromine	g/m ³		2.9
Dissolved Calcium	g/m ³		30
Dissolved Copper	g/m ³		0.040
Dissolved Iron	g/m ³		22
Dissolved Magnesium	g/m ³		5
Dissolved Manganese	g/m ³		1.41
Total Nickel*	g/m ³		0.167
Total Potassium*	g/m ³		40
Total Sodium*	g/m ³		790
Total Sulphur	g/m ³		11
Total Zinc*	g/m ³		0.040
Chloride	g/m ³		750
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		33
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		104
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		12.3
Toluene	g/m ³		6.4
Ethylbenzene	g/m ³		0.23
m&p-Xylene	g/m ³		1.25
o-Xylene	g/m ³		0.49




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 7 return HF Fluid	
Lab Number:	3152661.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	1.04
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	16.0
C10 - C14	g/m ³	36
C15 - C36	g/m ³	24
Total hydrocarbons (C7 - C36)	g/m ³	76

3152661.4
 Composite of Turangi 14 Stim 7 return HF Fluid
 Client Chromatogram for TPH by FID

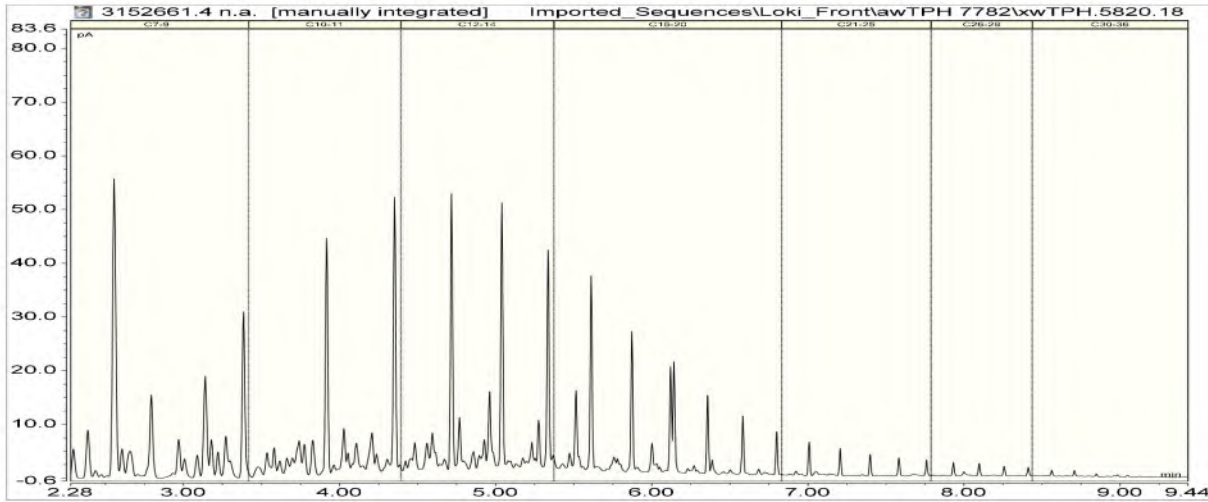

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 18-Jan-2023 and 24-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3152662	SPV1
Contact:	Fiona Campbell	Date Received:	17-Jan-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	26-Jan-2023	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	258066	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 6 Return HF Fluid		
Lab Number:	3152662.3		
Individual Tests			
pH	pH Units		6.6
Total Alkalinity	g/m ³ as CaCO ₃		900
Total Hardness	g/m ³ as CaCO ₃		195
Electrical Conductivity (EC)	mS/m		354
Salinity*			1.7
Total Suspended Solids	g/m ³		430
Total Dissolved Solids (TDS)	g/m ³		2,900
Dissolved Barium	g/m ³		3.0
Dissolved Bromine	g/m ³		1.7
Dissolved Calcium	g/m ³		70
Dissolved Copper	g/m ³		0.125
Dissolved Iron	g/m ³		17.8
Dissolved Magnesium	g/m ³		5
Dissolved Manganese	g/m ³		0.85
Total Nickel*	g/m ³		0.39
Total Potassium*	g/m ³		44
Total Sodium*	g/m ³		610
Total Sulphur	g/m ³		22
Total Zinc*	g/m ³		0.29
Chloride	g/m ³		590
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		67
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		12.6
Toluene	g/m ³		15.0
Ethylbenzene	g/m ³		1.62
m&p-Xylene	g/m ³		10.2
o-Xylene	g/m ³		3.6



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.


Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 6 Return HF Fluid	
Lab Number:	3152662.3	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	138
C10 - C14	g/m ³	430
C15 - C36	g/m ³	470
Total hydrocarbons (C7 - C36)	g/m ³	1,030

3152662.3

Composite of Turangi 14 Stim 6 Return HF Fluid

Client Chromatogram for TPH by FID

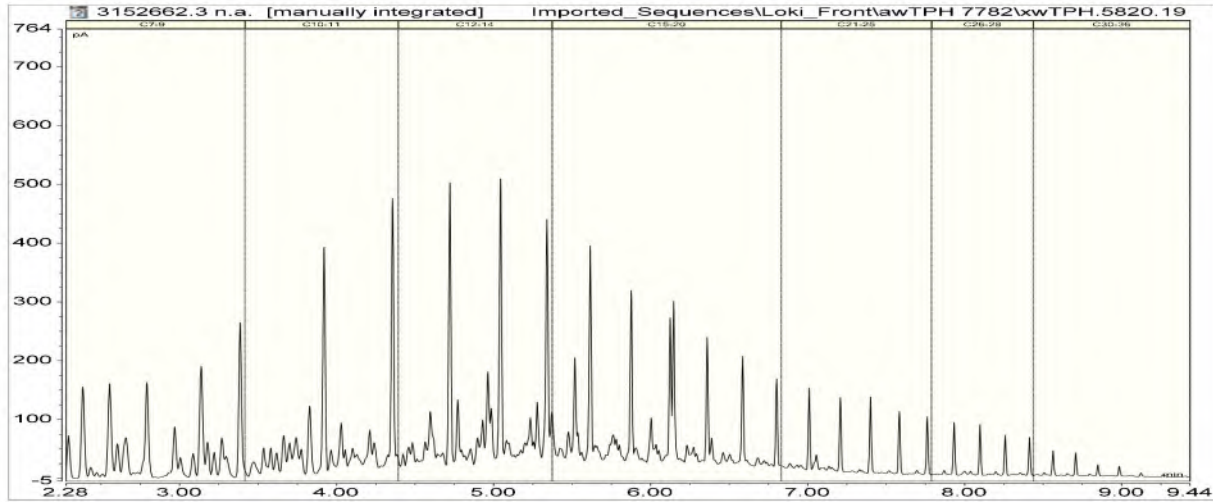**Analyst's Comments**

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	3
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	3
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	3
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	3
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	3
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	3

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	3
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	3
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	3
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	3
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	3
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	3
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	3
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	3
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	3
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	3
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	3
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	3
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	3
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	3
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	3
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	3
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	3
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	3
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	3
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	3
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	3
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	3
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	3
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	3
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	3
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	3
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	3

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 18-Jan-2023 and 26-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3140111	SPV1
Contact:	Fiona Campbell	Date Received:	19-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	30-Dec-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	257900	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 5 Return HF Fluid		
Lab Number:	3140111.4		
Individual Tests			
pH	pH Units		7.2
Total Alkalinity	g/m ³ as CaCO ₃		2,700
Total Hardness	g/m ³ as CaCO ₃		114
Electrical Conductivity (EC)	mS/m		916
Salinity*			5.2
Total Suspended Solids	g/m ³		250
Total Dissolved Solids (TDS)	g/m ³		7,900
Dissolved Barium	g/m ³		17.3
Dissolved Bromine	g/m ³		4.6
Dissolved Calcium	g/m ³		36
Dissolved Copper	g/m ³		0.027
Dissolved Iron	g/m ³		2.4
Dissolved Magnesium	g/m ³		6
Dissolved Manganese	g/m ³		0.20
Total Nickel*	g/m ³		0.048
Total Potassium*	g/m ³		60
Total Sodium*	g/m ³		2,200
Total Sulphur	g/m ³		9
Total Zinc*	g/m ³		0.052
Chloride	g/m ³		1,650
Nitrite-N	g/m ³		< 0.10
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10
Sulphate*	g/m ³		28
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		161
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		13.0
Toluene	g/m ³		24
Ethylbenzene	g/m ³		3.4
m&p-Xylene	g/m ³		20
o-Xylene	g/m ³		6.8




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 5 Return HF Fluid	
Lab Number:	3140111.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	0.91
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	230
C10 - C14	g/m ³	520
C15 - C36	g/m ³	500
Total hydrocarbons (C7 - C36)	g/m ³	1,260

3140111.4
 Composite of Turangi 14 Stim 5 Return HF Fluid
 Client Chromatogram for TPH by FID

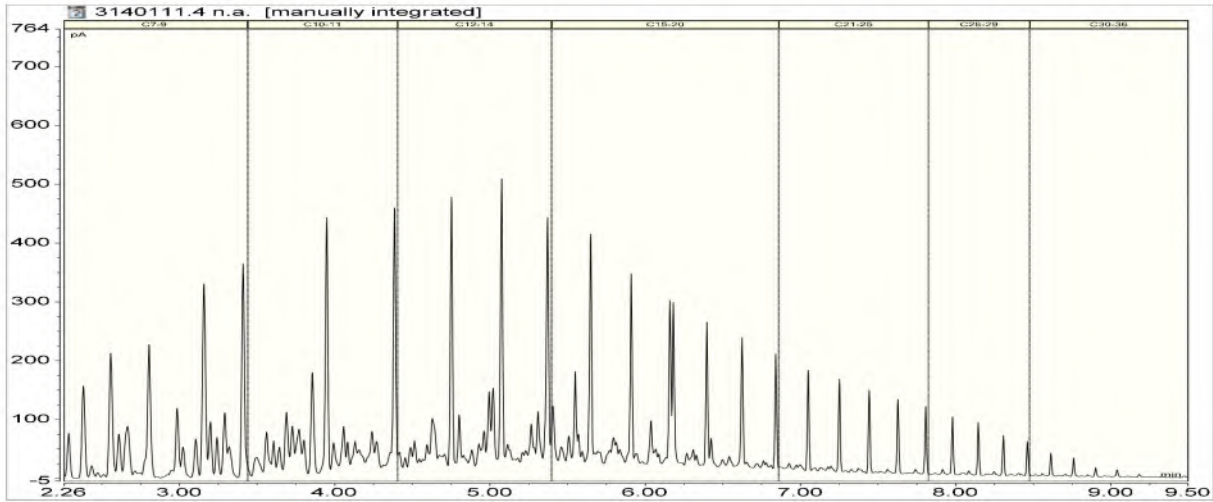

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Dec-2022 and 30-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3140110	SPV1
Contact:	Fiona Campbell	Date Received:	19-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	30-Dec-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	257846	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 4 Return Fluid		
Lab Number:	3140110.4		
Individual Tests			
pH	pH Units		6.6
Total Alkalinity	g/m ³ as CaCO ₃		1,070
Total Hardness	g/m ³ as CaCO ₃		310
Electrical Conductivity (EC)	mS/m		1,794
Salinity*			11.3
Total Suspended Solids	g/m ³		620
Total Dissolved Solids (TDS)	g/m ³		11,900
Dissolved Barium	g/m ³		44
Dissolved Bromine	g/m ³		17.3
Dissolved Calcium	g/m ³		101
Dissolved Copper	g/m ³		0.037
Dissolved Iron	g/m ³		9.4
Dissolved Magnesium	g/m ³		13
Dissolved Manganese	g/m ³		1.07
Total Nickel*	g/m ³		0.21
Total Potassium*	g/m ³		131
Total Sodium*	g/m ³		4,300
Total Sulphur	g/m ³		9
Total Zinc*	g/m ³		0.112
Chloride	g/m ³		5,800
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		27
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		39
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		14.4
Toluene	g/m ³		21
Ethylbenzene	g/m ³		2.2
m&p-Xylene	g/m ³		12.8
o-Xylene	g/m ³		3.9




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 14 Stim 4 Return Fluid	
Lab Number:	3140110.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	174
C10 - C14	g/m ³	230
C15 - C36	g/m ³	270
Total hydrocarbons (C7 - C36)	g/m ³	670

3140110.4
 Composite of Turangi 14 Stim 4 Return Fluid
 Client Chromatogram for TPH by FID

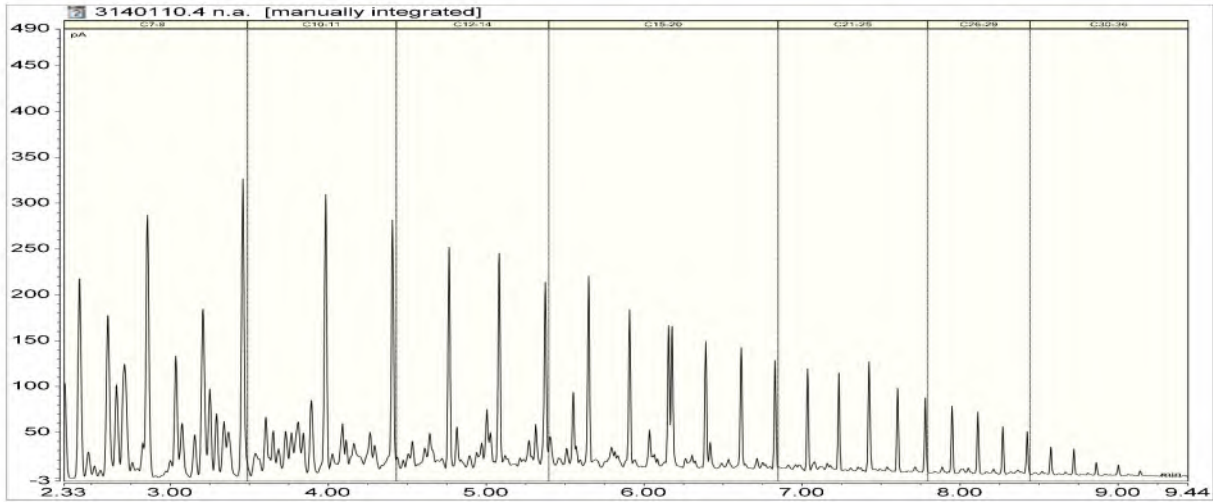

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Dec-2022 and 30-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3098711	SPV1
Contact:	Fiona Campbell	Date Received:	19-Oct-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	27-Oct-2022	
	14 Connett Road West	Quote No:	81870	
	Bell Block	Order No:	257172	
	New Plymouth 4312	Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous


Sample Name:	Composite of Turangi 14 Stim #3 Return Fluid		
Lab Number:	3098711.4		
Individual Tests			
pH	pH Units		6.6
Total Alkalinity	g/m ³ as CaCO ₃		760
Total Hardness	g/m ³ as CaCO ₃		410
Electrical Conductivity (EC)	mS/m		1,920
Salinity*			11.2
Total Suspended Solids	g/m ³		250
Total Dissolved Solids (TDS)	g/m ³		13,600
Dissolved Barium	g/m ³		28
Dissolved Bromine	g/m ³		21
Dissolved Calcium	g/m ³		133
Dissolved Copper	g/m ³		0.45
Dissolved Iron	g/m ³		5.8
Dissolved Magnesium	g/m ³		18
Dissolved Manganese	g/m ³		2.9
Total Nickel*	g/m ³		0.44
Total Potassium*	g/m ³		128
Total Sodium*	g/m ³		3,900
Total Sulphur	g/m ³		10
Total Zinc*	g/m ³		0.20
Chloride	g/m ³		5,400
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		30
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		27
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		10.8
Toluene	g/m ³		8.1
Ethylbenzene	g/m ³		0.57
m&p-Xylene	g/m ³		2.8
o-Xylene	g/m ³		1.13



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous		
Sample Name:	Composite of Turangi 14 Stim #3 Return Fluid	
Lab Number:	3098711.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	51
C10 - C14	g/m ³	126
C15 - C36	g/m ³	168
Total hydrocarbons (C7 - C36)	g/m ³	340

3098711.4
Composite of Turangi 14 Stim #3 Return Fluid
Client Chromatogram for TPH by FID

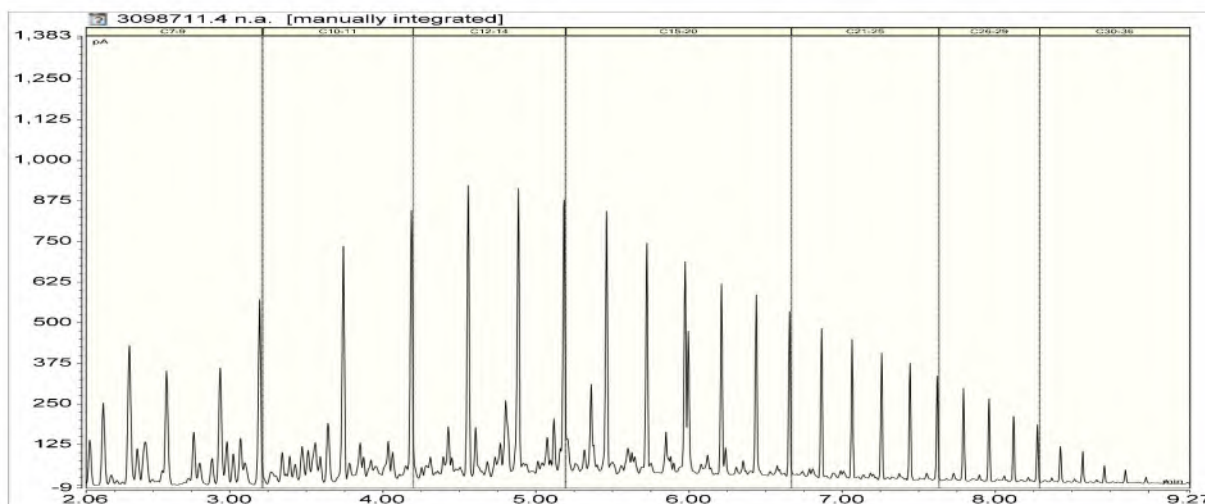

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 22-Oct-2022 and 27-Oct-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized strokes that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	2704224	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	15-Sep-2021	
		Date Reported:	23-Sep-2021	
		Quote No:	81870	
		Order No:	253943	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Composite of Turangi 14 Strim 2 Return Fluid Start, Turangi 14 Strim 2 Return Fluid Middle & Turangi 14 Strim 2 Return Fluid End				
Lab Number:	2704224.4				

Individual Tests

pH*	pH Units	6.9	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	700	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	440	-	-	-	-
Electrical Conductivity (EC)*	mS/m	1,856	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	12,200	-	-	-	-
Dissolved Barium	g/m ³	41	-	-	-	-
Dissolved Bromine	g/m ³	18.4	-	-	-	-
Dissolved Calcium	g/m ³	150	-	-	-	-
Dissolved Copper	g/m ³	0.027	-	-	-	-
Dissolved Iron	g/m ³	1.94	-	-	-	-
Dissolved Magnesium	g/m ³	16	-	-	-	-
Dissolved Manganese	g/m ³	5.5	-	-	-	-
Total Nickel	g/m ³	0.198	-	-	-	-
Total Potassium	g/m ³	240	-	-	-	-
Total Sodium	g/m ³	3,900	-	-	-	-
Total Sulphur*	g/m ³	14	-	-	-	-
Total Zinc	g/m ³	0.142	-	-	-	-
Chloride*	g/m ³	6,100	-	-	-	-
Nitrite-N	g/m ³	0.067	-	-	-	-
Nitrate-N	g/m ³	0.024	-	-	-	-
Nitrate*	g/m ³	0.11	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	0.091	-	-	-	-
Sulphate*	g/m ³	42	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	172	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.


Sample Type: Saline

Sample Name:	Composite of Turangi 14 Strim 2 Return Fluid Start, Turangi 14 Strim 2 Return Fluid Middle & Turangi 14 Strim 2 Return Fluid End				
Lab Number:	2704224.4				

BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	171	-	-	-	-
Toluene*	g/m ³	260	-	-	-	-
Ethylbenzene*	g/m ³	29	-	-	-	-
m&p-Xylene*	g/m ³	172	-	-	-	-
o-Xylene*	g/m ³	51	-	-	-	-
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	< 0.15	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	3,600	-	-	-	-
C10 - C14*	g/m ³	6,200	-	-	-	-
C15 - C36*	g/m ³	5,100	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	14,900	-	-	-	-

2704224.4

Composite of Turangi 14 Strim 2 Return Fluid Start, Turangi 14 Strim 2 Return Fluid Middle & Turangi 14 Strim 2 Return Fluid End
Client Chromatogram for TPH by FID

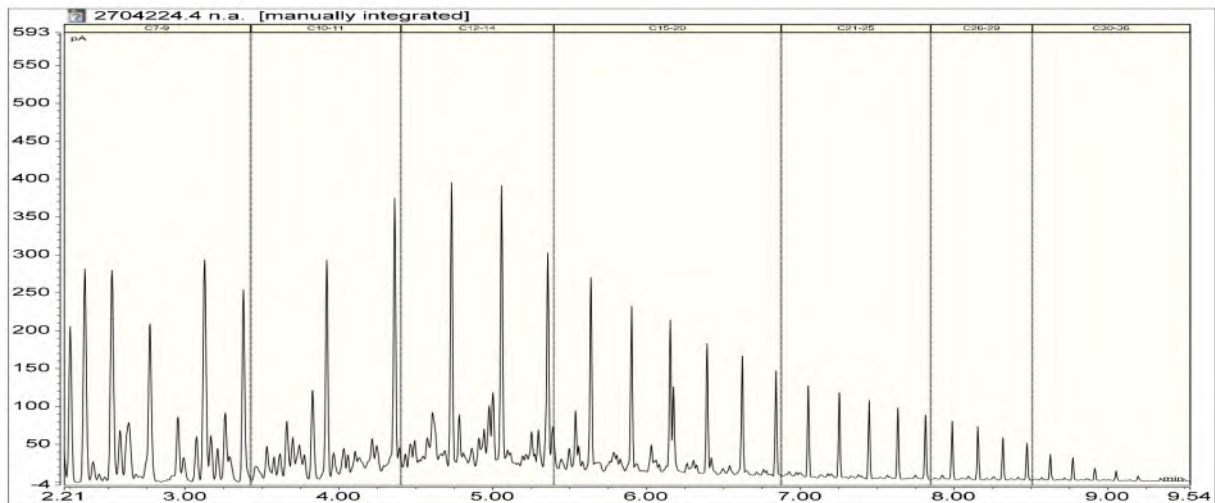

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 17-Sep-2021 and 23-Sep-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping loops and lines, positioned above the name of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2707021	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	17-Sep-2021	
		Date Reported:	29-Sep-2021	
		Quote No:	81870	
		Order No:	253819	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi 14 Strim 1 Return HF Fluid				
Lab Number:	2707021.4				

Individual Tests

pH*	pH Units	7.1	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	930	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	230	-	-	-	-
Electrical Conductivity (EC)*	mS/m	1,471	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	10,900	-	-	-	-
Dissolved Barium	g/m ³	32	-	-	-	-
Dissolved Bromine	g/m ³	16.6	-	-	-	-
Dissolved Calcium	g/m ³	78	-	-	-	-
Dissolved Copper	g/m ³	0.031	-	-	-	-
Dissolved Iron	g/m ³	2.7	-	-	-	-
Dissolved Magnesium	g/m ³	9	-	-	-	-
Dissolved Manganese	g/m ³	3.3	-	-	-	-
Total Nickel	g/m ³	0.125	-	-	-	-
Total Potassium	g/m ³	194	-	-	-	-
Total Sodium	g/m ³	2,800	-	-	-	-
Total Sulphur*	g/m ³	13	-	-	-	-
Total Zinc	g/m ³	0.42	-	-	-	-
Chloride*	g/m ³	4,400	-	-	-	-
Nitrite-N	g/m ³	0.064	-	-	-	-
Nitrate-N	g/m ³	< 0.010	-	-	-	-
Nitrate*	g/m ³	< 0.05	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	0.063	-	-	-	-
Sulphate*	g/m ³	40	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	153	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-
BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	63	-	-	-	-
Toluene*	g/m ³	100	-	-	-	-
Ethylbenzene*	g/m ³	22	-	-	-	-
m&p-Xylene*	g/m ³	135	-	-	-	-
o-Xylene*	g/m ³	39	-	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:		Turangi 14 Strim 1 Return HF Fluid				
Lab Number:		2707021.4				
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	< 0.15	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	3,800	-	-	-	-
C10 - C14*	g/m ³	5,700	-	-	-	-
C15 - C36*	g/m ³	4,200	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	13,700	-	-	-	-

2707021.4
Turangi 14 Strim 1 Return HF Fluid
Client Chromatogram for TPH by FID

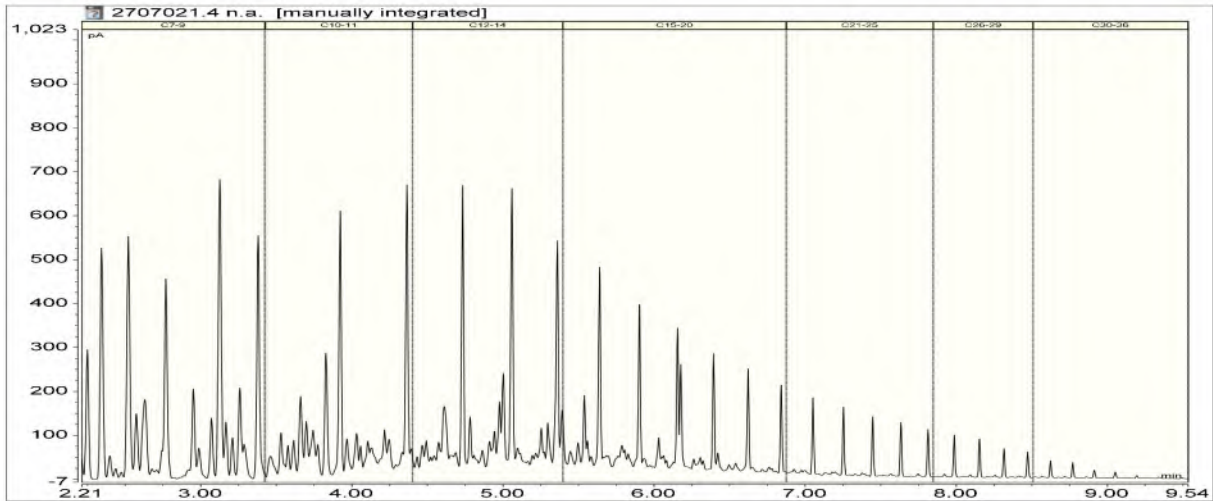

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ -I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ -I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 21-Sep-2021 and 29-Sep-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Carole Rodgers-Carroll BA, NZCS
Client Services Manager - Environmental




Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3150073	SPV1
Contact:	Fiona Campbell	Date Received:	12-Jan-2023	
	C/- Greymouth Petroleum Limited	Date Reported:	17-Jan-2023	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258260	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Turangi14 Stim 7 Prepumped HF Fluid 21-Dec-2022	
Lab Number:	3150073.1	
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	71
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	0.0027
Toluene	g/m ³	0.0119
Ethylbenzene	g/m ³	0.0018
m&p-Xylene	g/m ³	0.013
o-Xylene	g/m ³	0.0049
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	< 0.2
C10 - C14	g/m ³	< 0.4
C15 - C36	g/m ³	2.7
Total hydrocarbons (C7 - C36)	g/m ³	3.1

3150073.1
Turangi14 Stim 7 Prepumped HF Fluid 21-Dec-2022
Client Chromatogram for TPH by FID

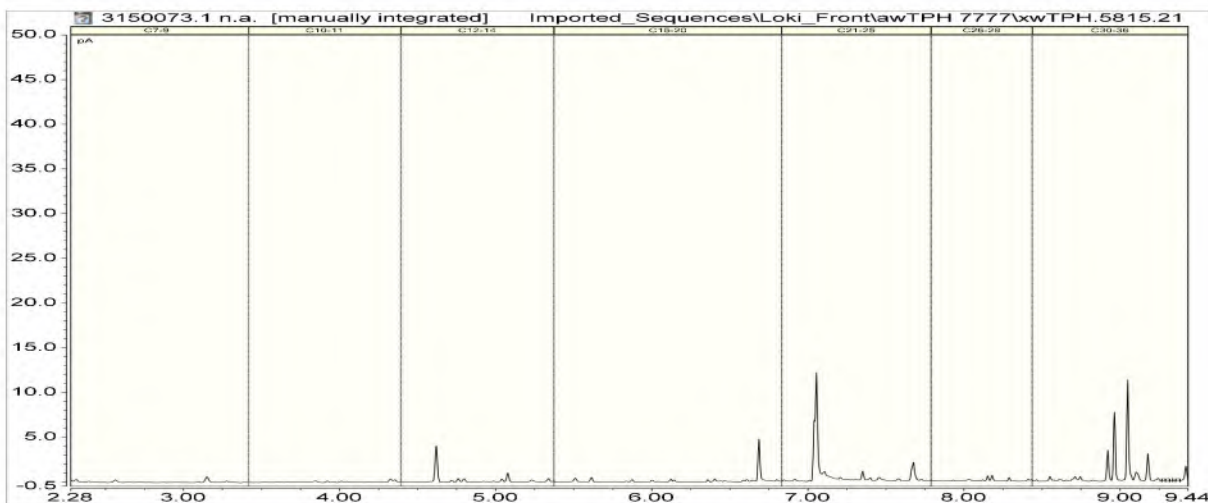

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 16-Jan-2023 and 17-Jan-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3139749	SPV1
Contact:	Fiona Campbell	Date Received:	17-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	22-Dec-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	258066	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 14 Stim6 Prepumped HF Fluid 15-Dec-2022		
Lab Number:	3139749.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	95	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0014	
Toluene	g/m ³	0.0102	
Ethylbenzene	g/m ³	0.0017	
m&p-Xylene	g/m ³	0.011	
o-Xylene	g/m ³	0.0040	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 20-Dec-2022 and 22-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3133699	SPV1
Contact:	Fiona Campbell	Date Received:	09-Dec-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	22-Dec-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	257900	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 14 Stim 5 Prepumped HF Fluid 07-Dec-2022		
Lab Number:	3133699.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	730	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0023	
Toluene	g/m ³	0.0148	
Ethylbenzene	g/m ³	0.0018	
m&p-Xylene	g/m ³	0.015	
o-Xylene	g/m ³	0.0058	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 13-Dec-2022 and 22-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental




Certificate of Analysis

Page 1 of 2

Client:	Greymouth Petroleum Limited	Lab No:	3124345	SPV1
Contact:	Fiona Campbell	Date Received:	26-Nov-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	02-Dec-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	257846	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous			
Sample Name:	Turangi 14 Stim #4 Prepumped HF Fluid 23-Nov-2022		
Lab Number:	3124345.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		760
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		< 20
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		0.0026
Toluene	g/m ³		0.0149
Ethylbenzene	g/m ³		0.0020
m&p-Xylene	g/m ³		0.015
o-Xylene	g/m ³		0.0057
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³		< 0.5
C10 - C14	g/m ³		< 1.0
C15 - C36	g/m ³		2
Total hydrocarbons (C7 - C36)	g/m ³		< 4

3124345.1
Turangi 14 Stim #4 Prepumped HF Fluid 23-Nov-2022
Client Chromatogram for TPH by FID

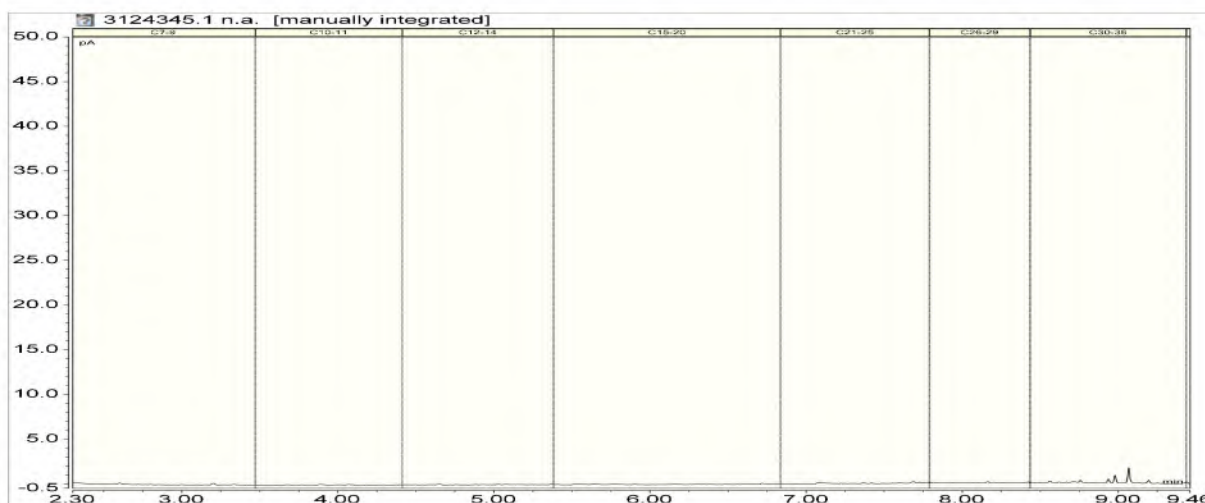

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 29-Nov-2022 and 02-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3088604	SPV1
Contact:	Fiona Campbell	Date Received:	04-Oct-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	13-Oct-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	257172	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 14 Stim #3 Prepumped HF Fluid 28-Sep-2022		
Lab Number:	3088604.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	560	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0124	
Toluene	g/m ³	0.056	
Ethylbenzene	g/m ³	0.0059	
m&p-Xylene	g/m ³	0.043	
o-Xylene	g/m ³	0.0146	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	< 2	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1



This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 07-Oct-2022 and 13-Oct-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2704278	SPV1
Contact:	Fiona Campbell	Date Received:	15-Sep-2021	
	C/- Greymouth Petroleum Limited	Date Reported:	22-Sep-2021	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	253943	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	


Sample Type: Aqueous

Sample Name:	Turangi 14 Stim 2 Prepumped HF Fluid 08-Sep-2021					
Lab Number:	2704278.1					
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	< 20	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-
BTEX in Water by Headspace GC-MS						
Benzene	g/m ³	< 0.010	-	-	-	-
Toluene	g/m ³	0.018	-	-	-	-
Ethylbenzene	g/m ³	< 0.010	-	-	-	-
m&p-Xylene	g/m ³	< 0.02	-	-	-	-
o-Xylene	g/m ³	< 0.010	-	-	-	-
Total Petroleum Hydrocarbons in Water						
C7 - C9	g/m ³	2.1	-	-	-	-
C10 - C14	g/m ³	2,800	-	-	-	-
C15 - C36	g/m ³	135	-	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	2,900	-	-	-	-

2704278.1

Turangi 14 Stim 2 Prepumped HF Fluid 08-Sep-2021

Client Chromatogram for TPH by FID

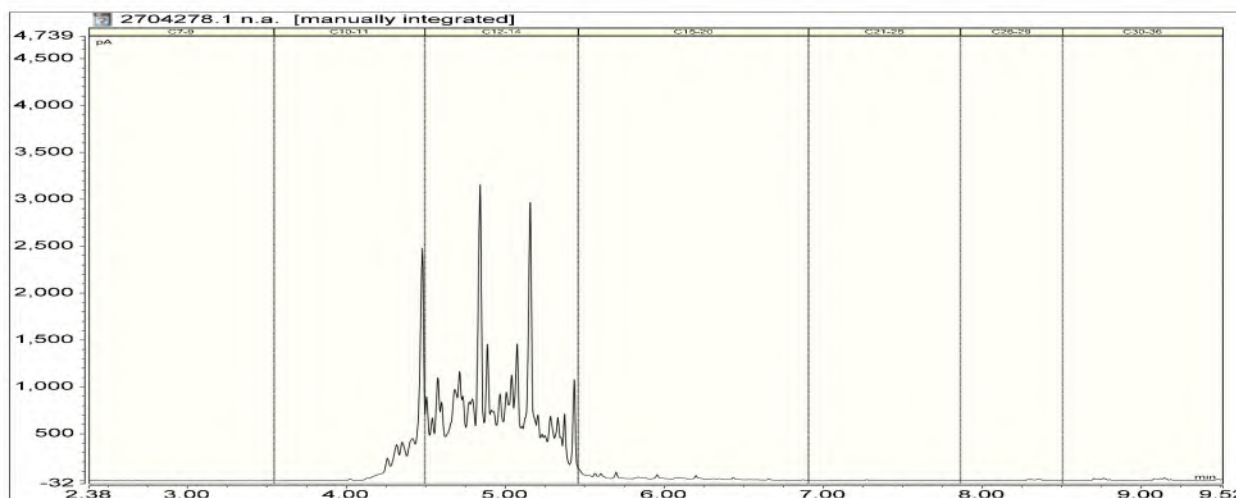

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 17-Sep-2021 and 22-Sep-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Martin Cowell - BSc
Client Services Manager - Environmental



Certificate of Analysis


Client:	Greymouth Petroleum Limited	Lab No:	2698594	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	09-Sep-2021	
		Date Reported:	21-Sep-2021	
		Quote No:	85159	
		Order No:	253819	
		Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 14 Stim 1 Prepumped HF Fluid 02-Sep-2021				
Lab Number:	2698594.1				

Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	< 20	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	0.008	-	-	-
Toluene	g/m ³	0.038	-	-	-
Ethylbenzene	g/m ³	< 0.008	-	-	-
m&p-Xylene	g/m ³	0.026	-	-	-
o-Xylene	g/m ³	0.009	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	5	-	-	-
C10 - C14	g/m ³	4,100	-	-	-
C15 - C36	g/m ³	350	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	4,400	-	-	-

2698594.1
Turangi 14 Stim 1 Prepumped HF Fluid 02-Sep-2021
Client Chromatogram for TPH by FID

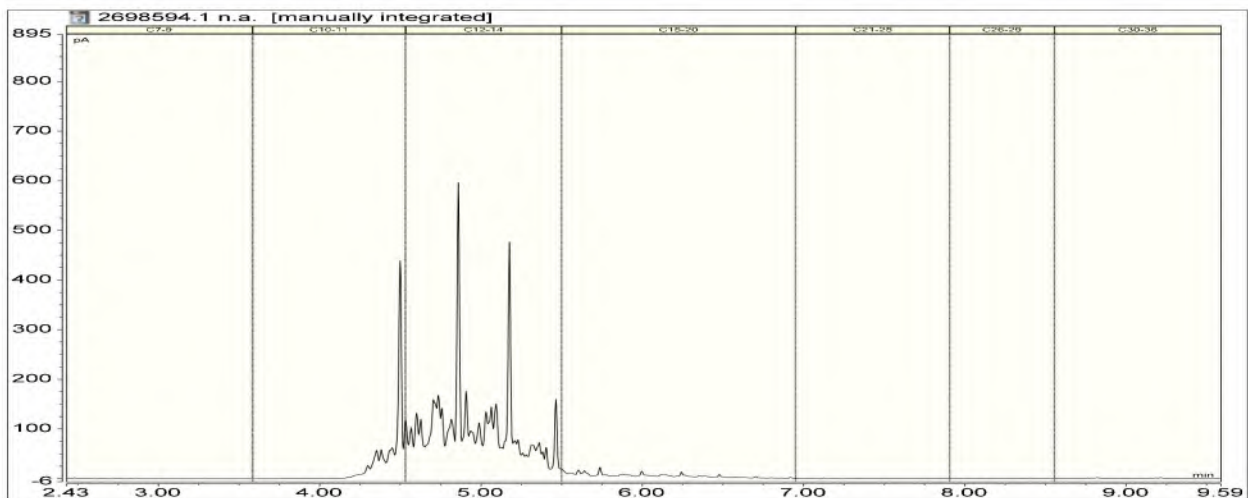

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 14-Sep-2021 and 21-Sep-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3122361	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	24-Nov-2022	
		Date Reported:	02-Dec-2022	
		Quote No:	81870	
		Order No:	257758	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Composite of Turangi 11 Stim#8 Return HF Fluid		
Lab Number:	3122361.4		
Individual Tests			
pH	pH Units		6.9
Total Alkalinity	g/m ³ as CaCO ₃		1,440
Total Hardness	g/m ³ as CaCO ₃		280
Electrical Conductivity (EC)	mS/m		1,878
Salinity*			11.1
Total Suspended Solids	g/m ³		490
Total Dissolved Solids (TDS)	g/m ³		12,600
Dissolved Barium	g/m ³		40
Dissolved Bromine	g/m ³		17.4
Dissolved Calcium	g/m ³		89
Dissolved Copper	g/m ³		< 0.005
Dissolved Iron	g/m ³		5.2
Dissolved Magnesium	g/m ³		13
Dissolved Manganese	g/m ³		4.9
Total Nickel*	g/m ³		0.22
Total Potassium*	g/m ³		146
Total Sodium*	g/m ³		4,000
Total Sulphur	g/m ³		7
Total Zinc*	g/m ³		0.153
Chloride	g/m ³		5,900
Nitrite-N	g/m ³		< 0.10 #1
Nitrate-N	g/m ³		< 0.10
Nitrate	g/m ³		< 0.5
Nitrate-N + Nitrite-N	g/m ³		< 0.10 #1
Sulphate*	g/m ³		21
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³		< 20
Propylene Glycol in Water*			
Propylene glycol*	g/m ³		< 20
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³		400
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³		17.9
Toluene	g/m ³		28
Ethylbenzene	g/m ³		2.6
m&p-Xylene	g/m ³		16.7
o-Xylene	g/m ³		5.3




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Aqueous

Sample Name:	Composite of Turangi 11 Stim#8 Return HF Fluid	
Lab Number:	3122361.4	
Formaldehyde in Water by DNPH & LCMSMS		
Formaldehyde	g/m ³	< 0.15
Total Petroleum Hydrocarbons in Water		
C7 - C9	g/m ³	260
C10 - C14	g/m ³	580
C15 - C36	g/m ³	400
Total hydrocarbons (C7 - C36)	g/m ³	1,240

3122361.4
 Composite of Turangi 11 Stim#8 Return HF Fluid
 Client Chromatogram for TPH by FID

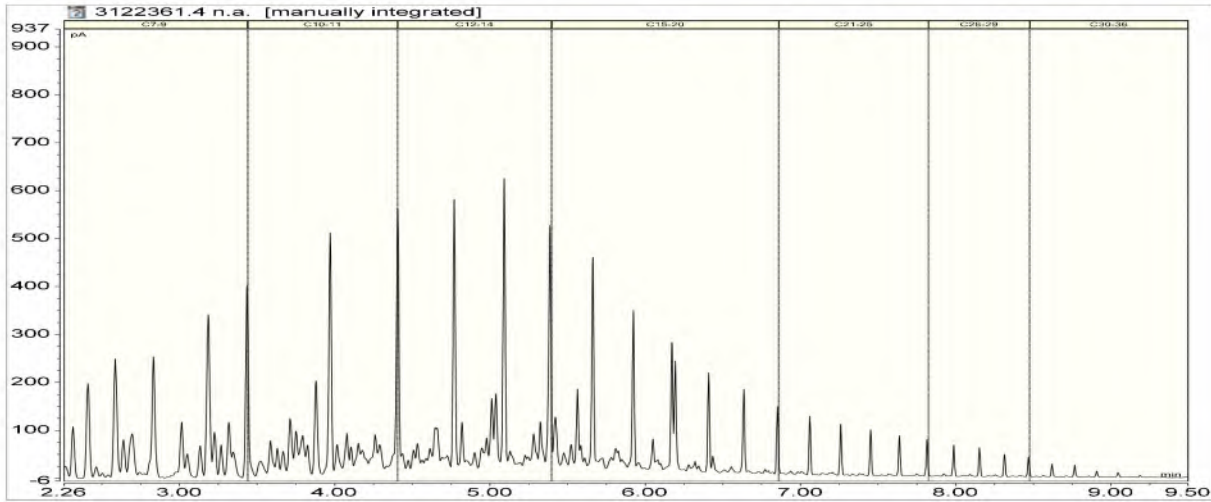

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 26-Nov-2022 and 02-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

A handwritten signature in blue ink, consisting of several overlapping, stylized lines that form a unique, illegible mark.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	2673316	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	07-Aug-2021	
		Date Reported:	16-Aug-2021	
		Quote No:	81870	
		Order No:	253545	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Saline

Sample Name:	Turangi II Stim 7 Return HF Fluid				
Lab Number:	2673316.4				

Individual Tests

pH*	pH Units	8.2	-	-	-	-
Total Alkalinity*	g/m ³ as CaCO ₃	1,460	-	-	-	-
Total Hardness*	g/m ³ as CaCO ₃	128	-	-	-	-
Electrical Conductivity (EC)*	mS/m	6,040	-	-	-	-
Total Dissolved Solids (TDS)*	g/m ³	5,400	-	-	-	-
Dissolved Barium	g/m ³	2.3	-	-	-	-
Dissolved Bromine	g/m ³	5.5	-	-	-	-
Dissolved Calcium	g/m ³	42	-	-	-	-
Dissolved Copper	g/m ³	0.005	-	-	-	-
Dissolved Iron	g/m ³	10.1	-	-	-	-
Dissolved Magnesium	g/m ³	6	-	-	-	-
Dissolved Manganese	g/m ³	3.3	-	-	-	-
Total Nickel	g/m ³	0.41	-	-	-	-
Total Potassium	g/m ³	185	-	-	-	-
Total Sodium	g/m ³	1,250	-	-	-	-
Total Sulphur*	g/m ³	11	-	-	-	-
Total Zinc	g/m ³	0.036	-	-	-	-
Chloride*	g/m ³	1,180	-	-	-	-
Nitrite-N	g/m ³	< 0.05	-	-	-	-
Nitrate-N	g/m ³	0.05	-	-	-	-
Nitrate*	g/m ³	0.2	-	-	-	-
Nitrate-N + Nitrite-N	g/m ³	0.08	-	-	-	-
Sulphate*	g/m ³	34	-	-	-	-
Ethylene Glycol in Water*						
Ethylene glycol*	g/m ³	121	-	-	-	-
Propylene Glycol in Water*						
Propylene glycol*	g/m ³	< 20	-	-	-	-
Methanol in Water - Aqueous Solvents*						
Methanol*	g/m ³	< 20	-	-	-	-
BTEX in Water by Headspace GC-MS*						
Benzene*	g/m ³	10.0	-	-	-	-
Toluene*	g/m ³	6.2	-	-	-	-
Ethylbenzene*	g/m ³	0.23	-	-	-	-
m&p-Xylene*	g/m ³	1.21	-	-	-	-
o-Xylene*	g/m ³	0.50	-	-	-	-




This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Sample Type: Saline

Sample Name:		Turangi II Stim 7 Return HF Fluid				
Lab Number:		2673316.4				
Formaldehyde in Water by DNPH & LCMSMS*						
Formaldehyde*	g/m ³	< 0.15	-	-	-	-
Total Petroleum Hydrocarbons in Water*						
C7 - C9*	g/m ³	16.0	-	-	-	-
C10 - C14*	g/m ³	104	-	-	-	-
C15 - C36*	g/m ³	52	-	-	-	-
Total hydrocarbons (C7 - C36)*	g/m ³	173	-	-	-	-

2673316.4
Turangi II Stim 7 Return HF Fluid
Client Chromatogram for TPH by FID

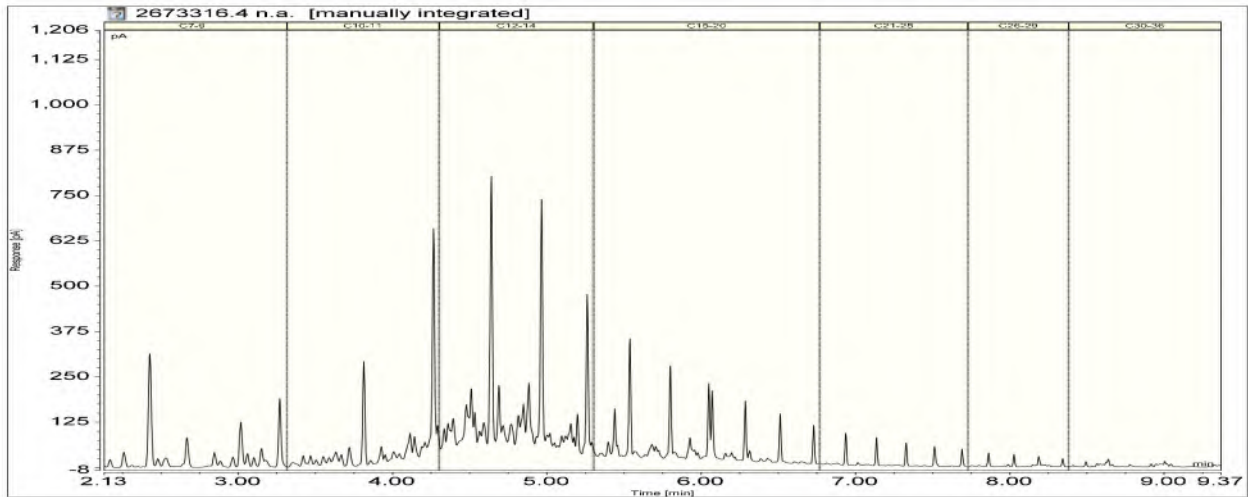

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Saline

Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved*	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion*	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH*	pH meter. APHA 4500-H+ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity*	Saline water, Titration to pH 4.5.	1.0 g/m ³ as CaCO ₃	4
Total Hardness*	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)*	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Total Dissolved Solids (TDS)*	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis*	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4

Sample Type: Saline			
Test	Method Description	Default Detection Limit	Sample No
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur*	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc	Nitric acid digestion, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride*	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate*	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS*	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS*	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36*	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)*	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 10-Aug-2021 and 16-Aug-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental




Certificate of Analysis

Client:	Greymouth Petroleum Limited	Lab No:	3119372	SPV1
Contact:	Fiona Campbell	Date Received:	19-Nov-2022	
	C/- Greymouth Petroleum Limited	Date Reported:	02-Dec-2022	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	257758	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 11 Stim #8 Prepumped HF Fluids 17-Nov-2022		
Lab Number:	3119372.1		
Ethylene Glycol in Water*			
Ethylene glycol*	g/m ³	720	
Propylene Glycol in Water*			
Propylene glycol*	g/m ³	< 20	
Methanol in Water - Aqueous Solvents*			
Methanol*	g/m ³	< 20	
BTEX in Water by Headspace GC-MS			
Benzene	g/m ³	0.0031	
Toluene	g/m ³	0.0183	
Ethylbenzene	g/m ³	0.0023	
m&p-Xylene	g/m ³	0.017	
o-Xylene	g/m ³	0.0064	
Total Petroleum Hydrocarbons in Water			
C7 - C9	g/m ³	< 0.5	
C10 - C14	g/m ³	< 1.0	
C15 - C36	g/m ³	3	
Total hydrocarbons (C7 - C36)	g/m ³	< 4	

3119372.1
Turangi 11 Stim #8 Prepumped HF Fluids 17-Nov-2022
Client Chromatogram for TPH by FID

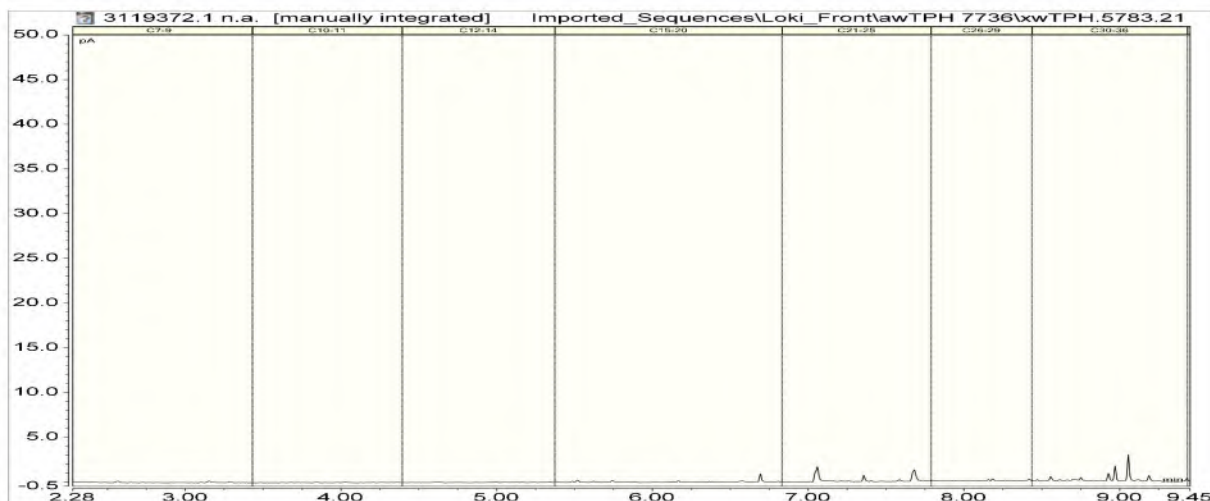

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 22-Nov-2022 and 02-Dec-2022. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.

Ara Heron BSc (Tech)
Client Services Manager - Environmental



Certificate of Analysis


Client:	Greymouth Petroleum Limited	Lab No:	2664273	SPV1
Contact:	Fiona Campbell	Date Received:	27-Jul-2021	
	C/- Greymouth Petroleum Limited	Date Reported:	30-Jul-2021	
	14 Connett Road West	Quote No:	85159	
	Bell Block	Order No:	253545	
	New Plymouth 4312	Client Reference:	Hydraulic fracturing fluid testing	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous

Sample Name:	Turangi 11 Stim7 Prepumped HF Fluids 23-Jul-2021				
Lab Number:	2664273.1				

Ethylene Glycol in Water*					
Ethylene glycol*	g/m ³	< 20	-	-	-
Propylene Glycol in Water*					
Propylene glycol*	g/m ³	< 20	-	-	-
Methanol in Water - Aqueous Solvents*					
Methanol*	g/m ³	< 20	-	-	-
BTEX in Water by Headspace GC-MS					
Benzene	g/m ³	0.0015	-	-	-
Toluene	g/m ³	0.0027	-	-	-
Ethylbenzene	g/m ³	< 0.0010	-	-	-
m&p-Xylene	g/m ³	< 0.002	-	-	-
o-Xylene	g/m ³	< 0.0010	-	-	-
Total Petroleum Hydrocarbons in Water					
C7 - C9	g/m ³	0.8	-	-	-
C10 - C14	g/m ³	3,500	-	-	-
C15 - C36	g/m ³	183	-	-	-
Total hydrocarbons (C7 - C36)	g/m ³	3,700	-	-	-

2664273.1
Turangi 11 Stim7 Prepumped HF Fluids 23-Jul-2021
Client Chromatogram for TPH by FID

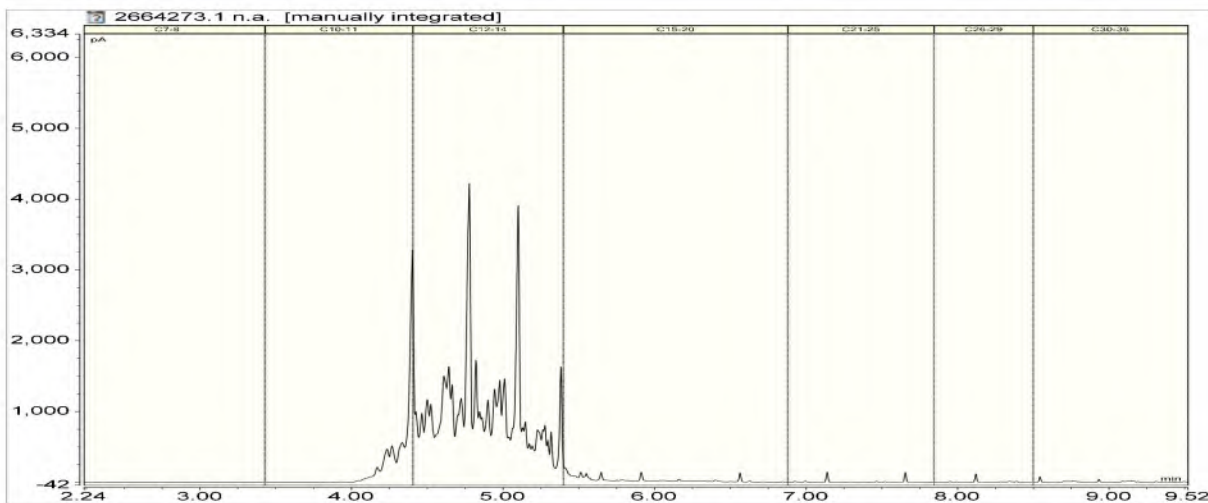

This Laboratory is accredited by International Accreditation New Zealand (IANZ), which represents New Zealand in the International Laboratory Accreditation Cooperation (ILAC). Through the ILAC Mutual Recognition Arrangement (ILAC-MRA) this accreditation is internationally recognised. The tests reported herein have been performed in accordance with the terms of accreditation, with the exception of tests marked * or any comments and interpretations, which are not accredited.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Laboratories, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	1
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	1
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	1
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	1
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	1
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	1
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	1

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 29-Jul-2021 and 30-Jul-2021. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Graham Corban MSc Tech (Hons)
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 4


Client:	Greymouth Petroleum Limited	Lab No:	3307063	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	22-Jun-2023	
		Date Reported:	06-Jul-2023	
		Quote No:	81870	
		Order No:	261037	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous		
Sample Name:	Composite of Turangi 19 Stim6 Return HF Fluid Start, Turangi 19 Stim6 Return HF Fluid Middle & Turangi 19 Stim6 Return HF Fluid End	
Lab Number:	3307063.4	
Individual Tests		
pH	pH Units	7.2
Total Alkalinity	g/m ³ as CaCO ₃	1,720
Total Hardness	g/m ³ as CaCO ₃	98
Electrical Conductivity (EC)	mS/m	867
Salinity*		4.8
Total Suspended Solids	g/m ³	600
Total Dissolved Solids (TDS)	g/m ³	7,400
Dissolved Barium	g/m ³	2.4
Dissolved Bromine	g/m ³	8.6
Dissolved Calcium	g/m ³	31
Dissolved Copper	g/m ³	0.023
Dissolved Iron	g/m ³	0.84
Dissolved Magnesium	g/m ³	5
Dissolved Manganese	g/m ³	0.68
Total Nickel*	g/m ³	0.049
Total Potassium*	g/m ³	61
Total Sodium*	g/m ³	1,850
Total Sulphur	g/m ³	12
Total Zinc*	g/m ³	0.081
Chloride	g/m ³	1,740
Nitrite-N	g/m ³	< 0.10 #1
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #1
Sulphate*	g/m ³	37
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	< 20
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 20
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	44
Toluene	g/m ³	84
Ethylbenzene	g/m ³	9.5
m&p-Xylene	g/m ³	58
o-Xylene	g/m ³	16.5

Sample Type: Aqueous	
Sample Name:	Composite of Turangi 19 Stim6 Return HF Fluid Start, Turangi 19 Stim6 Return HF Fluid Middle & Turangi 19 Stim6 Return HF Fluid End
Lab Number:	3307063.4
Formaldehyde in Water by DNPH & LCMSMS	
Formaldehyde	g/m ³ < 0.15
Total Petroleum Hydrocarbons in Water	
C7 - C9	g/m ³ 6,900
C10 - C14	g/m ³ 8,500
C15 - C36	g/m ³ 5,300
Total hydrocarbons (C7 - C36)	g/m ³ 21,000

3307063.4

Composite of Turangi 19 Stim6 Return HF Fluid Start, Turangi 19 Stim6 Return HF Fluid Middle & Turangi 19 Stim6 Return HF Fluid End
Client Chromatogram for TPH by FID

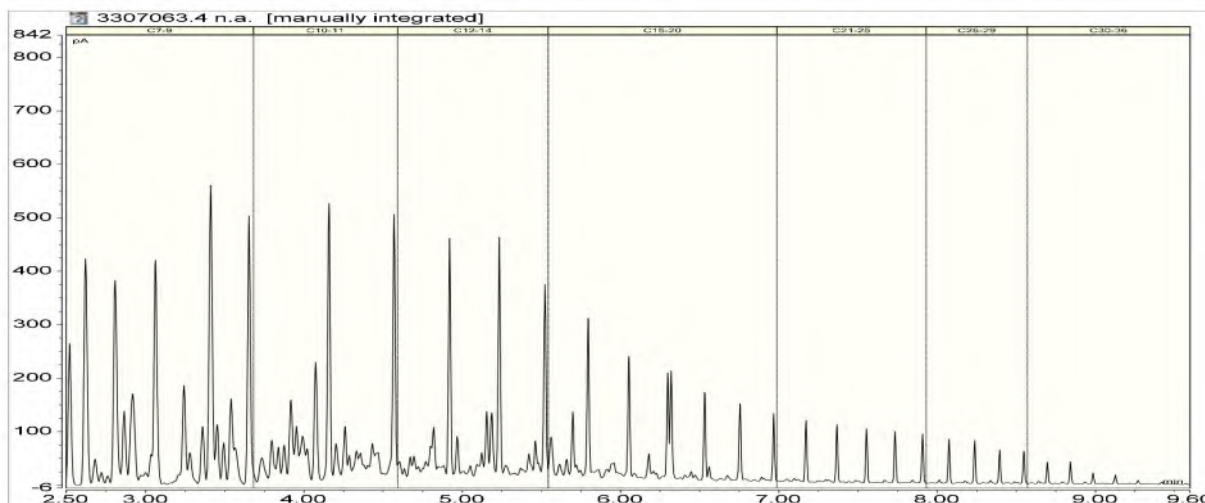

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 28-Jun-2023 and 06-Jul-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental

Certificate of Analysis

Page 1 of 4

Client:	Greymouth Petroleum Limited	Lab No:	3300278	SPV1
Contact:	Fiona Campbell C/- Greymouth Petroleum Limited 14 Connett Road West Bell Block New Plymouth 4312	Date Received:	13-Jun-2023	
		Date Reported:	23-Jun-2023	
		Quote No:	81870	
		Order No:	260929	
		Client Reference:	Return Fluid Composite	
		Submitted By:	Fiona Campbell	

Sample Type: Aqueous


Sample Name:	Composite of Turangi 19 Stim 5 Return HF Fluid Start, Turangi 19 Stim 5 Return HF Fluid Middle, Turangi 19 Stim 5 Return HF Fluid End
Lab Number:	3300278.4

Individual Tests		
pH	pH Units	7.7
Total Alkalinity	g/m ³ as CaCO ₃	2,100
Total Hardness	g/m ³ as CaCO ₃	96
Electrical Conductivity (EC)	mS/m	1,027
Salinity*		5.8
Total Suspended Solids	g/m ³	220
Total Dissolved Solids (TDS)	g/m ³	7,600
Dissolved Barium	g/m ³	4.5
Dissolved Bromine	g/m ³	10.8
Dissolved Calcium	g/m ³	29
Dissolved Copper	g/m ³	0.012
Dissolved Iron	g/m ³	2.3
Dissolved Magnesium	g/m ³	5
Dissolved Manganese	g/m ³	0.52
Total Nickel*	g/m ³	0.094
Total Potassium*	g/m ³	69
Total Sodium*	g/m ³	2,400
Total Sulphur	g/m ³	12
Total Zinc*	g/m ³	0.21
Chloride	g/m ³	2,300
Nitrite-N	g/m ³	< 0.10 #1
Nitrate-N	g/m ³	< 0.10
Nitrate	g/m ³	< 0.5
Nitrate-N + Nitrite-N	g/m ³	< 0.10 #1
Sulphate*	g/m ³	36
Ethylene Glycol in Water*		
Ethylene glycol*	g/m ³	39
Propylene Glycol in Water*		
Propylene glycol*	g/m ³	< 20
Methanol in Water - Aqueous Solvents*		
Methanol*	g/m ³	< 110
BTEX in Water by Headspace GC-MS		
Benzene	g/m ³	27
Toluene	g/m ³	27
Ethylbenzene	g/m ³	2.7
m&p-Xylene	g/m ³	14.4
o-Xylene	g/m ³	4.6

Sample Type: Aqueous	
Sample Name:	Composite of Turangi 19 Stim 5 Return HF Fluid Start, Turangi 19 Stim 5 Return HF Fluid Middle, Turangi 19 Stim 5 Return HF Fluid End
Lab Number:	3300278.4
Formaldehyde in Water by DNPH & LCMSMS	
Formaldehyde	g/m ³ < 1.5
Total Petroleum Hydrocarbons in Water	
C7 - C9	g/m ³ 250
C10 - C14	g/m ³ 340
C15 - C36	g/m ³ 330
Total hydrocarbons (C7 - C36)	g/m ³ 920

3300278.4

Composite of Turangi 19 Stim 5 Return HF Fluid Start, Turangi 19 Stim 5 Return HF Fluid Middle, Turangi 19 Stim 5 Return HF Fluid End
Client Chromatogram for TPH by FID

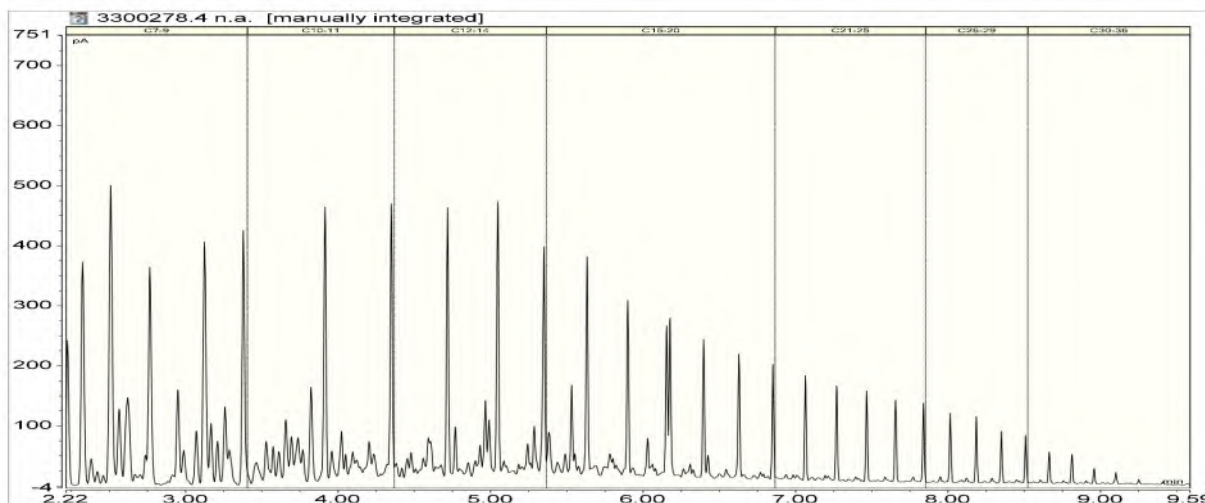

Analyst's Comments

#1 Due to the nature of this sample a dilution was performed prior to analysis, resulting in a detection limit higher than that normally achieved for the NO₂N, NO₃N and NO_xN analysis.

Summary of Methods

The following table(s) gives a brief description of the methods used to conduct the analyses for this job. The detection limits given below are those attainable in a relatively simple matrix. Detection limits may be higher for individual samples should insufficient sample be available, or if the matrix requires that dilutions be performed during analysis. A detection limit range indicates the lowest and highest detection limits in the associated suite of analytes. A full listing of compounds and detection limits are available from the laboratory upon request. Unless otherwise indicated, analyses were performed at Hill Labs, 28 Duke Street, Frankton, Hamilton 3204.

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Individual Tests			
Filtration, Unpreserved	Sample filtration through 0.45µm membrane filter.	-	4
Total Digestion	Boiling nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
Total Digestion of Saline Samples*	Nitric acid digestion. APHA 3030 E (modified) 23 rd ed. 2017.	-	4
pH	pH meter. APHA 4500-H ⁺ B 23 rd ed. 2017. Note: It is not possible to achieve the APHA Maximum Storage Recommendation for this test (15 min) when samples are analysed upon receipt at the laboratory, and not in the field. Samples and Standards are analysed at an equivalent laboratory temperature (typically 18 to 22 °C). Temperature compensation is used.	0.1 pH Units	4
Total Alkalinity	Titration to pH 4.5 (M-alkalinity), autotitrator. APHA 2320 B (modified for Alkalinity <20) 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Total Hardness	Calculation from Calcium and Magnesium. APHA 2340 B 23 rd ed. 2017.	1.0 g/m ³ as CaCO ₃	4
Electrical Conductivity (EC)	Conductivity meter, 25°C. APHA 2510 B 23 rd ed. 2017.	0.1 mS/m	4
Salinity*	Conductivity Meter (WTW Cond 340i with nonlinear temperature compensation according to EN 27 888). APHA 2520 B 23 rd ed. 2017.	0.2	4

Sample Type: Aqueous			
Test	Method Description	Default Detection Limit	Sample No
Total Suspended Solids	Saline sample. Filtration using Whatman 934 AH, Advantec GC-50 or equivalent filters (nominal pore size 1.2 - 1.5µm), gravimetric determination. APHA 2540 D (modified) 23 rd ed. 2017.	3 g/m ³	4
Total Dissolved Solids (TDS)	Filtration through GF/C (1.2 µm), gravimetric. APHA 2540 C (modified; drying temperature of 103 - 105°C used rather than 180 ± 2°C) 23 rd ed. 2017.	50 g/m ³	4
Filtration for dissolved metals analysis	Sample filtration through 0.45µm membrane filter and preservation with nitric acid. APHA 3030 B 23 rd ed. 2017.	-	4
Dissolved Barium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0006 g/m ³	4
Dissolved Bromine	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.10 g/m ³	4
Dissolved Calcium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.0 g/m ³	4
Dissolved Copper	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Dissolved Iron	Filtered sample, ICP-MS with dynamic reaction cell, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.004 g/m ³	4
Dissolved Magnesium	Filtered sample, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.4 g/m ³	4
Dissolved Manganese	Filtered sample, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0010 g/m ³	4
Total Nickel*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.0070 g/m ³	4
Total Potassium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	1.1 g/m ³	4
Total Sodium*	Nitric acid digestion, ICP-MS, ultratrace level. APHA 3125 B 23 rd ed. 2017.	0.42 g/m ³	4
Total Sulphur	Nitric acid digestion, ICP-OES (method may not fully account for H ₂ S due to volatilisation during digestion). All forms of oxidised and organic sulphur will be determined by this method. APHA 3120 B 23 rd ed. 2017.	0.5 g/m ³	4
Total Zinc*	Nitric acid digestion, ICP-MS, ultratrace. APHA 3125 B 23 rd ed. 2017.	0.0042 g/m ³	4
Chloride	Filtered sample. Ion Chromatography. APHA 4110 B (modified) 23 rd ed. 2017.	0.5 g/m ³	4
Nitrite-N	Saline sample. Automated Azo dye colorimetry, Flow injection analyser. APHA 4500-NO ₂ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Nitrate-N	Calculation: (Nitrate-N + Nitrite-N) - NO ₂ N. In-House.	0.0010 g/m ³	4
Nitrate	Calculation from Nitrate-N.	0.005 g/m ³	4
Nitrate-N + Nitrite-N	Saline sample. Total oxidised nitrogen. Automated cadmium reduction, Flow injection analyser. APHA 4500-NO ₃ ⁻ I (modified) 23 rd ed. 2017.	0.0010 g/m ³	4
Total Sulphate*	Calculation: from total sulphur.	2 g/m ³	4
Ethylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Propylene Glycol in Water*	Direct injection, dual column GC-FID.	4 g/m ³	4
Methanol in Water - Aqueous Solvents*	GC-FID analysis. In-house.	1.0 g/m ³	4
BTEX in Water by Headspace GC-MS	Headspace GC-MS analysis. In-house based on US EPA 8260 and 5021.	0.0010 - 0.002 g/m ³	4
Formaldehyde in Water by DNPH & LCMSMS	Derivatisation, SPE extraction, LC-MS/MS analysis. In-house based on US EPA 8315A.	0.02 g/m ³	4
Total Petroleum Hydrocarbons in Water			
C7 - C9	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.10 g/m ³	4
C10 - C14	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.2 g/m ³	4
C15 - C36	Solvent extraction, GC-FID analysis. In-house based on US EPA 8015.	0.4 g/m ³	4
Total hydrocarbons (C7 - C36)	Calculation: Sum of carbon bands from C7 to C36. In-house based on US EPA 8015.	0.7 g/m ³	4

These samples were collected by yourselves (or your agent) and analysed as received at the laboratory.

Testing was completed between 14-Jun-2023 and 23-Jun-2023. For completion dates of individual analyses please contact the laboratory.

Samples are held at the laboratory after reporting for a length of time based on the stability of the samples and analytes being tested (considering any preservation used), and the storage space available. Once the storage period is completed, the samples are discarded unless otherwise agreed with the customer. Extended storage times may incur additional charges.

This certificate of analysis must not be reproduced, except in full, without the written consent of the signatory.



Kim Harrison MSc
Client Services Manager - Environmental